

Data-Driven Variable Impedance Control of a Powered Knee-Ankle Prosthesis for Adaptive Speed and Incline Walking

T. Kevin Best, Cara Gonzalez Welker, Elliott J. Rouse, and Robert D. Gregg

Abstract—Most impedance-based walking controllers for powered knee-ankle prostheses use a finite state machine with dozens of user-specific parameters that require manual tuning by technical experts. These parameters are only appropriate near the task (*e.g.*, walking speed and incline) at which they were tuned, necessitating many different parameter sets for variable-task walking. In contrast, this paper presents a data-driven, phase-based controller for variable-task walking that uses continuously-variable impedance control during stance and kinematic control during swing to enable biomimetic locomotion. After generating a data-driven model of variable joint impedance with convex optimization, we implement a novel task-invariant phase variable and real-time estimates of speed and incline to enable autonomous task adaptation. Experiments with above-knee amputee participants (N=2) show that our data-driven controller 1) features highly-linear phase estimates and accurate task estimates, 2) produces biomimetic kinematic and kinetic trends as task varies, leading to low errors relative to able-bodied references, and 3) produces biomimetic joint work and cadence trends as task varies. We show that the presented controller meets and often exceeds the performance of a benchmark finite state machine controller for our two participants, without requiring manual impedance tuning.

Index Terms—Prostheses, Impedance Control, Optimization

I. INTRODUCTION

To perform activities that require net-positive energy, such as ascending ramps and stairs, passive prosthesis users must supply supplemental power from intact joints [1], leading to secondary complications including increased energy expenditure [2], osteoarthritis [3], [4], and lower back pain [5]. While powered prostheses can help avoid these complications by performing net-positive work [1], [6]–[9], designing prosthetic control systems for diverse environments remains a challenge.

Impedance control is a common strategy in lower-limb wearable robotics because of its simplicity and ability to produce behaviors that are similar to human biology, such as a compliantly controlled interaction with the ground [10] and dynamics similar to what has been observed in skeletal muscles [11]. Further, empirical studies have shown that ankle joint dynamics during walking are well described with an impedance controller [12]–[14]. A standard impedance con-

troller calculates joint torque τ based on a joint angle θ and joint velocity $\dot{\theta}$ as

$$\tau = -K(\theta - \theta_{\text{eq}}) - B\dot{\theta}, \quad (1)$$

where K , B , and θ_{eq} are parameters defining the joint's stiffness, damping, and equilibrium angle, respectively.

Traditional methods of impedance control for lower-limb prostheses involve segmenting the gait cycle into discrete sub-phases, where each sub-phase has its own constant values of K , B , and θ_{eq} . Researchers manually tune the impedance parameters in each sub-phase until the observed gait is satisfactory [6], [15]–[19]. Switching between sub-phases is controlled by a finite state machine (FSM) with transition criteria based on sensor readings (*e.g.*, elapsed time, leg loading, joint angles, etc.). Like the impedance parameters, these transition criteria are often experimentally tuned for an individual's gait by a technical expert. More elaborate impedance value representations have been suggested [19]–[22], but these methods still required manual, expert tuning.

Joint kinematics and kinetics vary based on the ground incline and walking speed [23], [24] (together termed the user's *task*). Therefore, the necessary impedance parameters and state machine transition criteria also vary. For a standard FSM impedance controller to operate over a wide array of tasks, many tunable parameters are required. For example, one multi-modal impedance controller required a total of 140 tunable parameters for five ambulation modes [20]. While only a portion of these parameters were considered necessary to tune, the device's configuration and tuning still required the researchers up to five hours to complete.

In contrast to the standard FSM-based impedance control paradigm, some authors have suggested using continuous functions to define the impedance parameters and how they evolve over the gait cycle [25]–[28]. In general, controllers that continually vary a robot's output mechanical impedance with time are known as variable impedance controllers [29]. Biomechanical principles suggest that human joints behave like variable impedance controllers [30] and empirical studies have observed this behavior at the ankle joint during walking [12]–[14]. Therefore, variable impedance control may offer a biomimetic solution for controlling powered prosthetic legs. However, how to appropriately define the variable impedance functions to realize walking gaits remains an open question.

A variable impedance controller was suggested in [26] using linear functions for stiffness and damping during stance. The linear functions were hand-tuned and held constant regardless of task. The variable impedance control method in [25] eliminated tuning altogether by using able-bodied kinematic data to generate continuous impedance parameter functions of gait phase. However, this method was limited to the knee

This work was supported by the National Institute of Child Health & Human Development of the NIH under Award Number R01HD094772. This work was also supported by the National Science Foundation under Award Numbers 1846969, 1949869, and 1949346. The content is solely the responsibility of the authors and does not necessarily represent the official views of the NIH or NSF.

T. Kevin Best, Cara G. Welker, and Robert D. Gregg are with the Department of Electrical Engineering and Computer Science and the Robotics Institute, University of Michigan, Ann Arbor, MI 48109. Elliott J. Rouse is with the Department of Mechanical Engineering and the Robotics Institute, University of Michigan, Ann Arbor, MI 48109. Contact: {tkbest, cgwelker, ejrouse, rdgregg}@umich.edu

joint, did not consider joint kinetics, and was never experimentally validated. Recently, [27] proposed a similar variable impedance controller where ankle stiffness and damping were defined as polynomials in gait phase, and the coefficients defining the polynomials were identified using constrained least squares with an able-bodied kinematic and kinetic dataset. The authors utilized piecewise-constant equilibrium angles and demonstrated continuous stiffness and damping expressions that produced satisfactory gait with a post-optimization tuning protocol. This work was later extended to include variable inclines and a phase variable parameterization of stiffness and damping based on the phase portrait of the thigh angle and its integral [28]. However, this phase variable is known to have challenges with non-steady walking [31], and changes in impedance associated with walking speed were not considered. The authors of [28] also note that their method of identifying the impedance parameters is non-convex, which does not guarantee a globally optimal solution [32] for their controller.

This paper addresses these limitations by presenting a new phase-based, task-adaptive walking controller built on a hybrid combination of continuously-variable impedance control during stance and kinematic control during swing (Fig. 1). First, we present a convex, data-driven framework to calculate stance phase joint stiffness, damping, and equilibrium angle as continuous functions of gait phase, walking speed, and incline from an able-bodied dataset [24] (Section III). Paired with an analogous model of swing joint kinematics [23], our hybrid controller adapts behavior across varying tasks based on real-time phase, speed, and incline estimates (Section IV). Next, we present an improved phase variable that avoids kinematic singularities and is robust to the diverse family of thigh trajectories associated with variable-task walking. Then, we perform validation experiments with two above-knee amputee (AKA) participants, demonstrating that the adaptive controller produces biomimetic trends in joint kinematics, kinetics, work, and cadence across varying tasks (Section V). Finally, we show that our presented controller meets or exceeds the performance of a hand-tuned benchmark FSM impedance controller in most tested metrics, suggesting that our optimized kinematic and impedance models sufficiently capture the key biomechanics of variable-task walking.

II. RELATED WORK

Many researchers have attempted to lessen the manual tuning burden of FSM impedance controllers in previous work. One common approach is to limit impedance control to the stance phase of gait and use kinematic control in swing phase, similar to our proposed architecture. Though many have used this hybrid architecture without a phase variable [6], [33]–[40], relatively few have used it with one [28], [41]. Phase variable parameterization can be helpful because it allows continuous regulation of the dynamic interaction between the user and the ground during stance and provides the user with indirect volitional control over foot position during swing [31].

Additionally, some researchers have used biological quasi-stiffness curves calculated from able-bodied data [33], [37], [38], [41], [42] in lieu of hand-tuned impedance parameters.

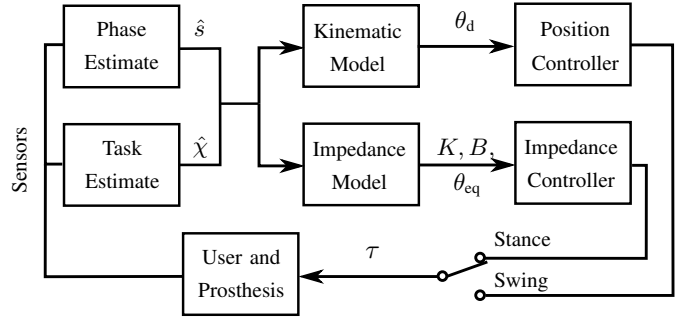


Fig. 1. A block diagram of the Hybrid Kinematic Impedance Controller presented in this work. Real-time estimates of gait phase \hat{s} and task $\hat{\chi}$ define desired joint impedance parameters K, B, θ_{eq} and joint angles θ_d using data-driven models. Depending on if the user is in stance or swing, the torque commands τ are calculated using either an impedance controller or a position controller, respectively.

While [33], [37], [38], [42] enabled variable-speed walking and [38] enabled obstacle crossing, these approaches were limited to level ground and relied on an FSM to switch between regions of the nonlinear quasi-stiffness curve during stance. Similarly, a quasi-passive ankle prosthesis presented in [43] enabled variable-incline walking with limited tuning by implementing a constant external quasi-stiffness relationship between the global shank angle and ankle torque. This external quasi-stiffness relationship was shown to be invariant across inclines during midstance, obviating the need for real-time incline estimation. However, this invariant relationship was limited to midstance and the controller relied on an FSM with manually tuned behavior for the remainder of the gait cycle. Further, as the control approach was developed for a passive prosthesis, it did not provide a method to increase net ankle work with increasing incline, which is an important characteristic of able-bodied walking [24]. Finally, this method was limited to ankle prostheses, and it is unclear whether the analogous external quasi-stiffness relationship for the knee during midstance is similarly invariant.

Other researchers have used reinforcement learning (RL) to automatically tune the impedance parameters online while a user walks, thus reducing the need for manual expert tuning [44]–[46]. Reward functions have been built on knee kinematic similarity to predefined trajectories or the observed contralateral knee’s trajectories. However, these approaches were limited to the knee joint only and can require several minutes of walking before the optimal impedance parameters are identified. Further, the RL algorithms focused on kinematic features; the resulting kinetics and overall biomechanics were not investigated.

Non-impedance-based tuning-free controllers have also been developed. In [31], [47], [48], able-bodied kinematic profiles parameterized by a phase variable (*i.e.*, virtual constraints) enabled tuning-free walking. This approach was extended for variable speed and incline walking in [49]. A similar controller was suggested for stair ascent [50]. However, the purely kinematic control paradigm tended to display non-biomimetic joint torques during stance. Additionally, the tuning-free knee-ankle prosthesis controller presented in [22] used an electromyography signal from the biceps femoris to control knee torque.

The ankle impedance controller used a constant stiffness and damping with an equilibrium angle calculated from the knee angle. This controller enabled walking, sitting, squatting, and lunging, but was not demonstrated on different slopes.

Finally, our work is most closely related to the phase-varying impedance controller derived from able-bodied data in [28], as discussed in Section I. However, our approach is distinct in multiple important ways. First, our convex optimization formulation provides an approximation of the globally optimal impedance parameter functions. In addition to global optimality, our convex formulation can be solved in polynomial time [32] to facilitate future work on real-time optimization using user data or clinician preference (e.g., [51]). Second, our variable impedance model includes a continuous function for equilibrium angle, mirroring the continuous progression of biological joint dynamics [12]–[14]. Third, our variable impedance model is further parameterized by walking speed, which is critical to reproducing normative gait energetics [48]. Fourth, we estimate the task variables in real-time, making the system fully autonomous. Fifth, we use a phase variable that is more robust to variable speed and incline behavior than prior phase variable definitions [28], [31], [48], [49]. And sixth, we demonstrate that our approach produces biomimetic trends in joint kinematics, kinetics, work, and cadence for two novel AKA participants over a range of tasks without any manual impedance tuning.

III. VARIABLE IMPEDANCE MODEL FOR STANCE

A. Model Framework

To use impedance control for the stance phase of the gait cycle in a continuous, phase-based control framework, we require a model analogous to the kinematic model developed in [23] that describes how the impedance parameters (K , B , and θ_{eq}) should evolve. Specifically, we require the impedance parameter model to be *continuously* parameterized by both gait phase s and task $\chi = (\nu, \gamma)$, where task is defined by the current walking speed ν and ground incline γ over the ranges $0.8 \leq \nu \leq 1.2$ m/s and $-10 \leq \gamma \leq 10$ deg.

A model that meets these criteria can be constructed from a linear combination of phase-varying polynomials, where the linear combination weights vary with the task. Polynomial functions of phase are useful to model parameter progression during stance because they are simply parameterized and can represent arbitrary aperiodic signals. We use fourth order polynomials ($d = 4$), as they allow sufficient flexibility to model the parameter behavior without overfitting. Once the appropriate polynomial functions are identified for individual tasks in a dataset, bilinear interpolation can be used to create a unified, continuous model with task and phase inputs.

First, we define task-specific polynomial functions that represent how the parameters vary during stance for a set of fixed tasks. For convenience, let s_{st} be the stance phase (i.e., $s_{\text{st}} = s/s_{\text{TO}}$, where s_{TO} is the phase at toe-off). Then, the impedance parameters for the p -th fixed task χ_p are

$$K_{\chi_p} = \sum_{i=0}^d k_{ip} s_{\text{st}}^i, \quad B_{\chi_p} = \sum_{i=0}^d b_{ip} s_{\text{st}}^i, \quad \theta_{\text{eq}, \chi_p} = \sum_{i=0}^d e_{ip} s_{\text{st}}^i, \quad (2)$$

where $\kappa_{\chi_p} = \{(k_{ip}, b_{ip}, e_{ip}) \mid i \in \{0, \dots, d\}\}$ is a set of constant coefficients. Then, the coefficients $\kappa_{\nu\gamma}$ defining the impedance parameter trajectories for an arbitrary task (ν, γ) are calculated through bilinear interpolation of its four nearest neighboring tasks κ_{ν_n, γ_n} , where $\nu_n \in \{\nu_1, \nu_2\}$, $\gamma_n \in \{\gamma_1, \gamma_2\}$. For all j elements in $\kappa_{\nu\gamma}$, this interpolation is

$$\kappa_{\nu\gamma}^j = \frac{[\nu_2 - \nu \quad \nu - \nu_1]}{(\nu_2 - \nu_1)(\gamma_2 - \gamma_1)} \begin{bmatrix} \kappa_{\nu_1 \gamma_1}^j & \kappa_{\nu_1 \gamma_2}^j \\ \kappa_{\nu_2 \gamma_1}^j & \kappa_{\nu_2 \gamma_2}^j \end{bmatrix} \begin{bmatrix} \gamma_2 - \gamma \\ \gamma - \gamma_1 \end{bmatrix}. \quad (3)$$

Finally, using $\kappa_{\nu\gamma}$ and (2) evaluated at the current stance phase s_{st} , the impedance parameters are calculated. Therefore, the model is fully defined once each task-specific set of coefficients κ_{χ_p} is calculated.

B. Model Fitting

We use an optimization-based approach to fit the model to a dataset of able-bodied walking [24]. The dataset contains kinematic and kinetic joint trajectories recorded from 10 participants walking at steady-state at 15 distinct points in the task space (i.e., $\gamma \in \{-10, -5, 0, 5, 10\}$ deg, $\nu \in \{0.8, 1.0, 1.2\}$ m/s). Therefore, for each task χ_p , we construct an optimization problem to identify the set of impedance parameter coefficients $\kappa_{\chi_p}^*$ that, when used in (1)–(2), best reproduced the mass-normalized joint torques τ in the dataset given the dataset kinematics $(\theta, \dot{\theta})$ over all n data points at χ_p :

$$\kappa_{\chi_p}^* = \arg \min_n \|\tau - \hat{\tau}\|_2^2, \quad (4)$$

$$\text{where } \hat{\tau} = K_{\chi_p} (\theta_{\text{eq}, \chi_p} - \theta) - B_{\chi_p} \dot{\theta}.$$

1) *Solution Approximation*: As written, (4) is difficult to solve, as the product $K_{\chi_p} \theta_{\text{eq}, \chi_p}$ is nonlinear in the unknown parameters, and the overall objective function is non-convex. To avoid this issue, we solve a similar, convex problem and use its solution to approximate a solution to (4). First, we combine the product of K_{χ_p} and $\theta_{\text{eq}, \chi_p}$ into a new, higher-order polynomial δ_{χ_p} with independent coefficients δ_{ip} :

$$K_{\chi_p} \theta_{\text{eq}, \chi_p} = \sum_{i=0}^d k_{ip} s_{\text{st}}^i \sum_{i=0}^d e_{ip} s_{\text{st}}^i = \sum_{i=0}^{2d} \delta_{ip} s_{\text{st}}^i = \delta_{\chi_p}. \quad (5)$$

By treating the δ_{ip} terms as independent from the k_{ip} terms, the impedance equation for $\hat{\tau}$ becomes linear in the unknown parameters k_{ip} , b_{ip} , and δ_{ip} . We can then write the modified optimization problem as a standard quadratic program (QP), defining a new argument vector $x \in \mathbb{R}^{4d+3 \times 1}$ as

$$x = [k_{0p}, \dots, k_{dp}, b_{0p}, \dots, b_{dp}, \delta_{0p}, \dots, \delta_{2dp}]^\top. \quad (6)$$

Let $\alpha_j \in \mathbb{R}^{4d+3 \times 1}$ be defined for each data point j as

$$\alpha_j = [-\theta_j s_j^0, \dots, -\theta_j s_j^d, -\dot{\theta}_j s_j^0, \dots, -\dot{\theta}_j s_j^d, s_j^0, \dots, s_j^{2d}]^\top. \quad (7)$$

Then, the objective function $L(\kappa_{\chi_p})$ from (4) becomes

$$L(\kappa_{\chi_p}) = \frac{1}{n} \|\tau - \hat{\tau}\|_2^2 = \frac{1}{n} \sum_{j=1}^n \tau_j^2 - f^\top x + \frac{1}{2} x^\top H x, \quad (8)$$

where

$$H = \frac{2}{n} \sum_{j=1}^n \alpha_j \alpha_j^\top, \quad f = \frac{2}{n} \sum_{j=1}^n \tau_j \alpha_j. \quad (9)$$

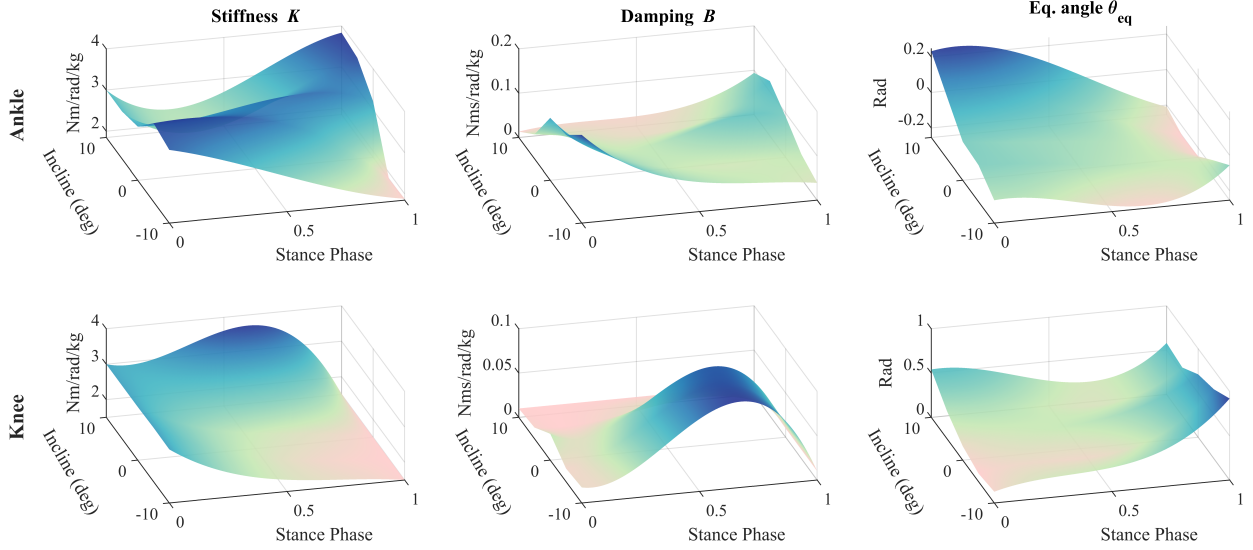


Fig. 2. Plots of the calculated impedance parameter functions, stiffness $K(s_{st}, \gamma, \nu)$, damping $B(s_{st}, \gamma, \nu)$, and equilibrium angle $\theta_{eq}(s_{st}, \gamma, \nu)$, for the knee and ankle, projected onto a speed of $\nu = 1$ m/s. These surfaces show the approximated solution to the original optimization problem (4).

2) *Constraints and Regularization*: To prevent overfitting, we added a diagonal regularization matrix $R = \text{diag}(\lambda) \in \mathbb{R}^{4d+3 \times 4d+3}$ to H to penalize the L_2 norm of x . The n -th diagonal entries in R corresponding to the regularization weights on k_i and b_i were $\lambda_n = 1e^{-5}$ while $\lambda_n = 1e^{-2}$ for the δ_i terms. These hyperparameters were chosen prior to the experiments in order to produce a smooth model that captured general behavior instead of overfitting to the training dataset.

Next, we added a constraint matrix A to ensure that $K_{\chi_p}(s)$ and $B_{\chi_p}(s)$ remained within ranges that were both physiologically realistic and feasible for the prosthesis to render in a stable manner. Namely, $K_{\chi_p}(s)$ was constrained above 1.5 Nm/rad/kg and $B_{\chi_p}(s)$ was constrained between 0.01 and 1.0 Nms/rad/kg. In addition, AKA participants in preliminary experiments noted that a low stiffness at heelstrike was unsettling, as they were accustomed to a locked knee during early stance with their take-home prostheses. Therefore, a minimum heelstrike stiffness constraint of 3.0 Nm/rad/kg was added to increase participants' confidence that the prosthesis was ready for weight acceptance at heelstrike.

To enforce these constraints, we discretized stance phase into n_j points in the range $[0, 1]$. We constructed a constraint matrix $A \in \mathbb{R}^{3n_j \times 4d+3}$ from sub-matrices $A_s \in \mathbb{R}^{n_j \times d+1}$ as

$$A_s = \begin{bmatrix} s_1^0 & \cdots & s_1^d \\ \vdots & \ddots & \vdots \\ s_{n_j}^0 & \cdots & s_{n_j}^d \end{bmatrix}, \quad A = \begin{bmatrix} -A_s & \mathbf{0} & \mathbf{0} \\ \mathbf{0} & -A_s & \mathbf{0} \\ \mathbf{0} & A_s & \mathbf{0} \end{bmatrix}. \quad (10)$$

A column vector $b \in \mathbb{R}^{3n_j \times 1}$ contained n_j copies of the minimum stiffness and damping and maximum damping values, with the first term modified for the heelstrike constraint:

$$b = -[3.0, 1.5, \dots, 1.5, 0.01, \dots, 0.01, -1.0, \dots, -1.0]^\top. \quad (11)$$

Finally, we arrived at the full QP, with the positive offset torque

(sum-of-squares) in (8) neglected without loss of generality:

$$\begin{aligned} & \underset{x}{\text{minimize}} && \frac{1}{2} x^\top (H + R)x - f^\top x \\ & \text{subject to} && Ax \leq b. \end{aligned} \quad (12)$$

We solved this QP for each subject and task χ_p combination in the dataset ($N = 150$) using the MATLAB Optimization Toolbox (R2021b, MathWorks, Natick, MA, USA). Then, we approximated the solution to the original problem (4) by projecting the rational function $\delta_{\chi_p}(s_{st})/K_{\chi_p}(s_{st}) = \theta_{eq, \chi_p}(s_{st})$ onto a d -th order polynomial. We assumed the polynomial order was sufficiently high to approximate the rational function $\delta_{\chi_p}(s_{st})/K_{\chi_p}(s_{st})$ without significant information loss. This assumption was validated by the model's low reconstruction error, detailed in the next section. Then for each task χ_p , the inter-subject mean set of coefficients $\bar{\kappa}_{\chi_p}$ was calculated for use as the final model. Trials that did not well-represent the data, measured by a Variance Accounted For (VAF) below 75%, were discarded as outliers prior to averaging.

C. Modeling Results

Fig. 2 shows the calculated impedance parameter model projected onto a speed of 1 m/s, which was produced by evaluating (2)-(3) with $\bar{\kappa}_{\chi_p}$. To quantify the impedance parameter model's reconstruction error, we calculated $\hat{\tau}$ for the knee and ankle over each trial in the dataset using the model:

$$\hat{\tau} = K(s_{st}, \gamma, \nu) (\theta_{eq}(s_{st}, \gamma, \nu) - \theta) - B(s_{st}, \gamma, \nu) \dot{\theta}. \quad (13)$$

Then, we calculated the root mean squared error (RMSE) in joint torque over all subjects for each task χ_p in the dataset and normalized by the dataset torque's standard deviation for χ_p . This dimensionless metric, which we call normalized reconstruction error \bar{E} , describes how many standard deviations $\hat{\tau}$ is from the mean dataset torque trajectories, on average. Normalized reconstruction errors below 1.0 indicate that the model is able to predict joint torque to accuracy levels similar

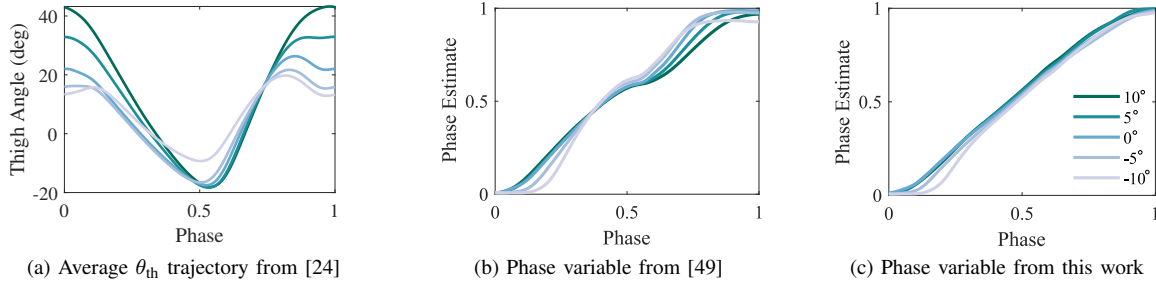


Fig. 3. Plots of (a) the mean able-bodied thigh trajectories reported in [24], where positive angles correspond to hip joint flexion, and (b)-(c) the resulting phase variable trajectories at different inclines. Plot (b) shows the trajectories calculated the previous method described in [49] and Plot (c) shows the trajectories calculated using the new phase variable presented in this work. The new method shows no phase pause near push-off and improved linearity, especially at the point of maximum hip extension.

to able-bodied inter-subject variation. Averaged over all tasks, the knee and ankle normalized reconstruction errors were $\bar{E}_k = 0.78 \pm 0.11$ and $\bar{E}_a = 0.58 \pm 0.09$, respectively.

IV. HYBRID KINEMATIC IMPEDANCE CONTROLLER

The proposed Hybrid Kinematic Impedance Controller (HKIC, Fig. 1) is an evolution of the purely kinematic controller presented in [49]. In the HKIC, real-time phase and task estimates provide inputs to the impedance model developed in Section III during stance and the kinematic model developed in [23] during swing to provide reference joint behavior. Impedance and position controllers enforce the respective model outputs, described below. Once configured with the user’s mass and leg segment lengths, the controller operates autonomously, requiring neither manual impedance tuning nor external knowledge of the terrain. The following paragraphs discuss each component of the HKIC in turn.

A. Task-Invariant Phase Estimation

An estimate of the user’s progression through the gait cycle is required in order to synchronize the control outputs with the user’s gait. An ideal version of this estimate (termed a *phase variable*) increases from 0 to 1 at a constant rate between each heelstrike [52]. Similar to [31], [49], the HKIC’s phase variable \hat{s} is calculated using a piecewise-linear mapping of the user’s global thigh angle θ_{th} , which has a roughly sinusoidal trajectory (see Fig. 3a). This angle is measured directly using an Inertial Measurement Unit (IMU, 3DM-CX5-25, LORD Microstrain, Williston, VT) mounted to the proximal end of the prosthesis’s knee joint. Mounting the IMU to the prosthesis instead of the person ensures a rigid connection to prevent slipping and vibration, which are commonly associated with soft tissue connections. Proper alignment of the prosthesis by a prosthetist ensures correct alignment of the IMU. The θ_{th} -based method of phase estimation is preferable because it allows the user to start and stop the gait cycle at will and enables non-rhythmic behavior [31].

However, previous iterations of the θ_{th} -based phase variable did not work well for variable-task locomotion because of assumptions made about the shape of the θ_{th} trajectory. For example, [31], [49] assumed that the θ_{th} trajectory could be divided into two monotonic sections. While this assumption holds fairly well for level ground and incline walking, it is

invalid for steep declines [24] (Fig. 3a). Previous methods produced inaccurate, saturated phase estimates for such cases [49]. Further, previous methods did not account for periods of low thigh angular velocity (*i.e.*, when the hip joint is most extended or most flexed), leading to pauses in the phase estimate and subsequent problems in the controller behavior [41], [49]. Therefore in this work, we relax previous assumptions and add flexibility to the phase variable to better parameterize the gait cycle based on the diverse θ_{th} trajectories observed in variable-task locomotion. First, we introduce short periods of feedforward phase progression that allow \hat{s} to maintain a constant positive rate even when thigh angular velocity is low, which enables a powerful and biomimetic push-off. Second, we add states to account for thigh trajectories that have more than two monotonic sections (especially common during ramp descent) to prevent excessive phase saturation and gait desynchronization. Third, we introduce a technique to improve the linearity of \hat{s} , correcting for previous steady-state nonlinearities and thus making it closer to an ideal phase estimate. For brevity, the mathematical details for these improvements are presented in Appendix A.

To illustrate the benefits of the new phase variable over its predecessor [31], [49], we conducted a simulation using thigh kinematic data from [24] (Fig. 3a). For each trial of treadmill walking in the dataset, we calculated the phase variable using both the new method (Appendix A) and the previous method described in [49]. For each incline, we averaged the phase trajectories over all strides, participants, and walking speeds, shown in Figs. 3b and 3c. Notably, the new phase variable eliminated the phase estimate pause associated with maximum hip extension that was observed with the previous phase variable. The new method also reduced the early saturation seen in the previous phase variable, which was particularly prominent at steep ramp declines. Finally, the new method demonstrated improved linearity, particularly during midstance. Compared to an ideal linear phase trajectory, the new method showed 6.25% RMSE with $R^2 = 0.990$ while the previous method showed 7.48% RMSE and $R^2 = 0.976$ over all tasks.

B. Task Estimation

In addition to the phase estimate, the HKIC requires an estimate of the user’s current task $\hat{\chi}$, which is calculated at each toe-off (TO) during steady walking. The estimation meth-

ods below are based on [49], with modifications to improve performance. Both estimates update once per stride and are filtered with a moving average over 3 strides to account for stride-to-stride variation. Although filtering introduces a time delay in the task estimates, experiments in [49] demonstrated that this limitation does not prevent the user from continuing to walk while the estimates converge.

1) *Walking Speed*: The user's speed is estimated using a three-link leg model, comprising thigh, shank, and foot links, similar to [33], [49], [53]–[55]. Using forward kinematics and inputs from the joint encoders and the thigh IMU, we calculate the Cartesian locations of the heel and toe relative to the hip joint, respectively given by x_{heel} and x_{toe} . At each TO event, the forward progression of the hip relative to the foot's point of contact with the ground during the previous stance phase is calculated as

$$d_{\text{st}} = \|x_{\text{toe}} - x_{\text{heel}}^{\text{HS-}}\|_2, \quad (14)$$

where $x_{\text{heel}}^{\text{HS-}}$ is the value of x_{heel} from the previous heelstrike (HS). Similarly by assuming a symmetric gait, the forward progression of the hip relative to the contralateral foot's ground contact point over a swing phase is approximated at each HS as

$$d_{\text{sw}} = \|x_{\text{heel}} - x_{\text{toe}}^{\text{TO-}}\|_2, \quad (15)$$

where $x_{\text{toe}}^{\text{TO-}}$ likewise is x_{toe} from the previous TO. Then, we calculate the total forward progression over the gait cycle as $d_{\text{st}} + d_{\text{sw}} + \ell_{\text{foot}}$, where ℓ_{foot} is a constant accounting for the length of the prosthetic foot. Finally, walking speed is estimated by dividing forward progression by stride time.

2) *Incline*: The ground inclination is estimated by the global angle of the foot θ_f when the foot was flat on the ground, similar to the methods presented in [16], [49], [54]–[56]. As it is undesirable to add an extra inertial sensor to the foot, we calculate this angle from the thigh IMU using forward kinematics, along with a correction for foot bending. Prosthetic feet are designed to deflect for energy storage [57], so foot deflection significantly impacts the incline estimate. Offline testing with our prosthesis's foot [39] (Lo Rider, 1E57, Ottobock, Duderstadt, Germany) showed that deflection was correlated with the bending moment in the sagittal plane m_y . An on-board 6-axis load cell (M3564F, Sunrise Instruments, Nanning, China), located at the distal end of the ankle joint, measures this moment directly. Then, θ_f is calculated as

$$\theta_f = \theta_{\text{th}} - \theta_{\text{k}} + \theta_{\text{a}} + \theta_{\text{f}}^0 + k_f m_y, \quad (16)$$

where k_f is the linear bending coefficient, θ_{k} is the relative knee angle, and θ_{a} is the relative ankle angle. All joint angles are measured positive in flexion and are zero when the user stands upright. The constant offset term θ_{f}^0 accounts for the angular difference between the prosthetic foot, the cosmesis, and the sole of the shoe.

To determine when the foot was flat on the ground, the center of pressure in the foot reference frame ℓ_{cop} is calculated using the load cell, similar to [49]. We consider the foot to be flat when $7.5 \leq \ell_{\text{cop}} \leq 12$ cm from the ankle joint, which corresponds to the ground reaction force acting between the middle and the ball of the foot. During this period, θ_f is averaged to produce the incline estimate for the stride.

C. Impedance and Kinematic Controllers

1) *Stance Impedance Controller*: During stance, a variable impedance controller is used to calculate joint torques. First, the stance phase estimate \hat{s}_{st} is calculated by

$$\hat{s}_{\text{st}} = \hat{s} / \bar{\hat{s}}_{\text{TO}}, \quad (17)$$

where $\bar{\hat{s}}_{\text{TO}}$ is the expected value of the phase variable at TO (see Appendix A for details). Using \hat{s}_{st} and $\hat{\chi}$, joint stiffness K , damping B , and equilibrium angle θ_{eq} are calculated using (2)–(3) and the model developed in Section III. Then, the joint torque during stance is calculated with the following impedance control law, scaled by user mass m :

$$\tau_{\text{st}} = m \left(K(\hat{s}_{\text{st}}, \hat{\chi})(\theta_{\text{eq}}(\hat{s}_{\text{st}}, \hat{\chi}) - \theta) - B(\hat{s}_{\text{st}}, \hat{\chi})\dot{\theta} \right). \quad (18)$$

2) *Swing Kinematic Controller*: A proportional derivative (PD) controller uses constant gains k_p and k_d to directly track desired joint angle trajectories. This is in contrast to the equilibrium angles of the impedance controller, which do not necessarily align with the normative joint angles. A continuous model of able-bodied joint kinematics [23], generated using data from [24], provides the desired trajectories defined as

$$\theta_{\text{d}}(s, \chi) = \sum_{i=1}^N b_k(s) c_k(\chi), \quad (19)$$

where $b_k(s)$ are Fourier series and $c_k(\chi)$ are Bernstein basis polynomials. Similar to the impedance model, (19) is evaluated in real-time using \hat{s} and $\hat{\chi}$. Then, the PD torque command during swing, τ_{sw} , is given by

$$\tau_{\text{sw}} = k_p(\theta_{\text{d}} - \theta) + k_d(\dot{\theta}_{\text{d}} - \dot{\theta}). \quad (20)$$

3) *Stance to Swing Transition Smoothing*: A time-varying weight w_{sw} ensures a smooth transition from impedance control to position control. Because impedance control may allow the joint angles to vary from their nominal trajectories depending on how the user loads the prosthesis, this smoothing is critical to avoid discrete changes in joint torque. At TO, w_{sw} increases from 0 to 1 over 0.25 s for the knee and 0.05 s for the ankle. The ankle smoothing is faster because close tracking of the ankle kinematics during early swing is important for avoiding toe-stubbing. The actual output to the joint motors is given by

$$\tau = \begin{cases} \tau_{\text{st}} & \text{during Stance,} \\ w_{\text{sw}} \tau_{\text{sw}} & \text{during Swing.} \end{cases} \quad (21)$$

Because the equilibrium angles at heelstrike are close to the kinematic references at the end of the gait cycle, no smoothing is necessary for the swing to stance transition.

Close examination of (21) shows that for a brief period just following TO, minimal control action is applied to the joints. This is acceptable because the low-impedance actuators used in our prosthesis [39] allow the joints to continue moving along their current trajectories according to their passive dynamics without control input. Passive early swing knee and ankle dynamics have been shown to produce human-like gait [58], [59], and these passive dynamics may contribute to the biomimetic behavior of the controller.

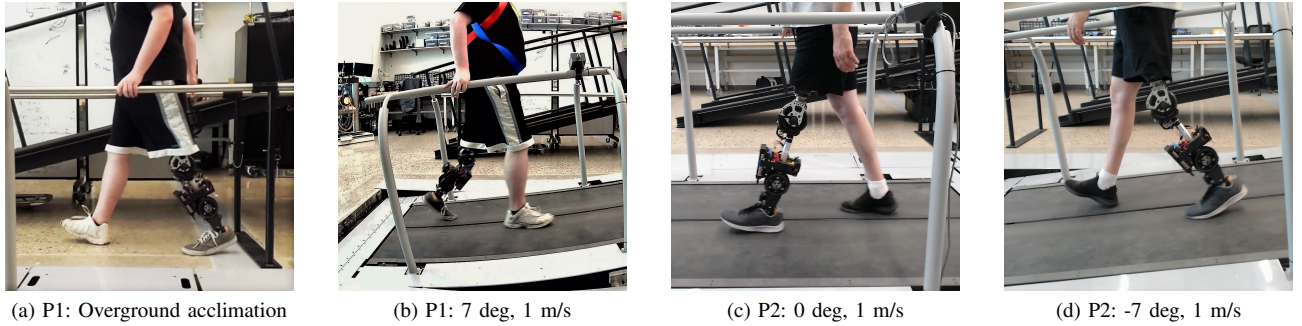


Fig. 4. Photos of above-knee amputee participants P1 and P2 performing various tasks with the HKIC during the experiments.

V. AMPUTEE PARTICIPANT EXPERIMENTS

Experiments with two AKA participants were performed to investigate the ability of the HKIC to produce biomimetic gaits over variable tasks. To benchmark the HKIC’s performance against another well-known controller, we also implemented a standard, piecewise-constant FSM impedance controller and tuned it for each participant. The participants completed the experimental protocol once with each controller, detailed below. Photos of the experiment are shown in Fig. 4 and video recordings are available for download as supplemental media.

A. Benchmark FSM Impedance Controller

A benchmark Finite State Machine controller (FSMC) was designed based on the variable-incline FSM impedance controller presented in [16], with an additional stance state and modified transition criteria to improve performance (see Appendix B for details). This controller was chosen as a benchmark because of its simple construction, widespread usage [1], and ability to create biomimetic walking gaits when appropriately tuned [16]. While more sophisticated variants of the FSM impedance control paradigm have shown stronger results, such as those that modulate the impedance parameters based on joint angles or prosthesis axial force [6], [20], [21], [60], [61], the original version from [16] provides a valuable benchmark for comparing novel controllers because its performance and limitations are widely understood [1], [9]. Further, many modern controllers still use FSM impedance control in some if not all sections of the gait cycle [18], [19], [34]–[36], [44]–[47], [62], so understanding the HKIC’s performance relative to the FSMC is scientifically relevant.

The FSMC had 5 discrete states throughout the gait cycle, each with its own set of constant impedance parameters and transition criteria. Similar to the methods discussed in the Introduction, these parameters needed to be hand-tuned by an expert researcher in order to produce the desired gait. To enable walking at various inclines, three sets of tunable impedance parameters and transition criteria were instantiated for each joint (*i.e.*, one set for level ground, one set for declines, and one set for inclines). The controller selected between impedance parameter sets based on the estimated incline $\hat{\gamma}$ (Appendix Fig. 15b). In total, the FSMC required 96 tunable parameters, including 45 impedance parameters per joint and 6 FSM transition criteria.

TABLE I
PARTICIPANT ATTRIBUTES

ID	Sex	Age (yrs)	Mass (kg)	Height (m)	Years since amputation	Etiology
P1	Male	26	116	1.9	26	Congenital
P2	Male	40	84	1.8	23	Cancer

B. Experimental Methods

Two AKA individuals participated in the experiment, with attributes shown in Table I. A third participant was enrolled but was unable to complete the protocol due to excessive swing-phase lateral whipping caused by prosthetic misalignment. Although we worked with the prosthetist to correct the alignment multiple times, the prosthesis would become misaligned again after a short walking bout, possibly due to a combination of his prosthetic socket and weak femur musculature [63]. We suspect that the large distal mass of the robotic prosthesis also exacerbated this problem. Due to this issue, we only present data from the remaining two subjects in this manuscript.

The experimental protocol was approved by the Institutional Review Board of the University of Michigan (HUM00166976), and the participants wore a ceiling-mounted safety harness while walking on the treadmill. For the experiments, the presented HKIC and the comparison FSMC were implemented on a backdrivable, powered knee-ankle prosthesis, shown in Fig. 4 and described in depth in [39]. This prosthesis features quasi-direct drive actuators that enable open-loop joint impedance control.

A licensed prosthetist fit the prosthesis to the participants and ensured proper alignment. The participants were instructed on the expected high-level behavior of both controllers and given time to acclimate to each controller while walking overground within parallel bars. Importantly, the participants were not told which controller was expected to perform better during the experiment. Following this overground acclimation, five trials with each controller were conducted on an in-ground treadmill (Bertec, Columbus, Ohio, USA). For safety, instrumented handrails were provided on either side of the treadmill. The participants were encouraged to limit body weight support on the handrails to maximize the realism of the experiment, which was verified by handrail force data. Participant P1’s mean handrail usage was under 12% body-weight and participant P2 frequently chose to use only one handrail (Fig. 4c-d).

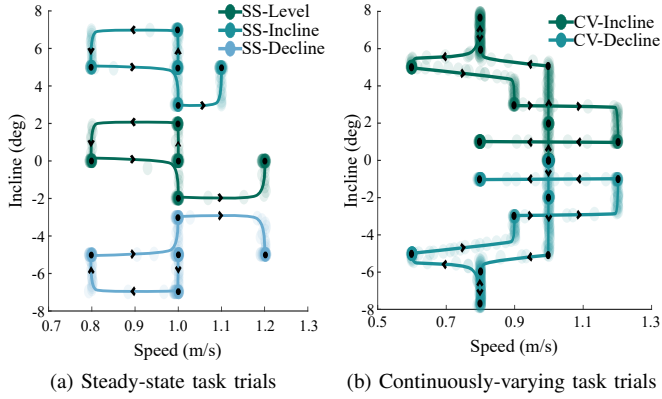


Fig. 5. Diagrams indicating the locations of the task space sampled during each trial. Each transparent marker indicates the treadmill’s task feedback, sampled at 2 Hz. Each black dot indicates the task combination commanded to the treadmill for a duration of 45 seconds in (a) and 20 seconds in (b).

The first three trials investigated the performance of the HKIC and the FSMC during steady walking at different speed and incline combinations. Each trial focused on a range of small task deviations (± 2 deg, ± 0.2 m/s) around one of three baseline tasks: $\chi = (0$ deg, 1 m/s), $\chi = (5$ deg, 1 m/s), and $\chi = (-5$ deg, 1 m/s). We refer to these steady-state task trials as SS-Level, SS-Incline, and SS-Dcline, respectively. For the SS-Incline trial, speed was limited to 1.1 m/s to ensure that the participants could safely perform the trial.

The steady-state task trials began with an acclimation period, where the participants walked at the baseline task until feeling comfortable. During this time, the FSMC was tuned by the authors of this work to produce a natural gait, incorporating feedback from the participants and the prosthetist. The authors have significant experience tuning impedance controllers [21], [47], [61]. Tuning continued until the authors, prosthetist, and participant were satisfied with the resulting natural gait (see Supplemental Video). The time taken to tune the FSMC was recorded. Note that no tuning was done for the HKIC. After tuning and acclimation, the participants walked on the treadmill as it cycled through each of the 5 tasks near the baseline task, each commanded for 45 seconds. In these trials, true task feedback was provided to the controllers so that any errors in the task estimates did not affect the results.

The tuning, acclimation and testing procedure above was repeated for each baseline task. These baseline tasks were chosen to be far apart in the task space in order to sample a wide range of tasks without deviating too far from any one of the FSMC’s tuning points. Fig. 5a shows the recorded task-space profiles from the treadmill for each trial, where the black dots indicate each commanded task.

The latter two trials consisted of more rapid task changes to investigate each controller’s behavior during continuous task variations rather than at steady-state and over a wider range of tasks. Also during these trials, the controllers received no real-time knowledge of the task from the treadmill, investigating the autonomous capability of each controller to operate over variable tasks. Both controllers utilized the same task estimation methods (Section IV-B). The FSMC transitioned between the tuned impedance parameters sets based on the

estimated incline (Appendix Fig. 15b). In these 2 trials, one with inclines (CV-Incline) and the other with declines (CV-Dcline), the treadmill started at $\chi = (0$ deg, 1 m/s) and explored 8 other points within the task space in the range of $[0, 8]$ deg and $[0.6, 1.2]$ m/s. Each task point was commanded to the treadmill for 20 seconds. Because the treadmill required time to change task, smooth task trajectories with continuous variations were generated, shown in Fig. 5b.

C. Experimental Results

1) *FSMC Tuning Time*: For the two participants, the FSMC required on average 30 min of tuning to produce normative gaits for the three baseline tasks. On average, the level ground task required 11 min, the incline task required 15 min, and the decline task required 5 min. Participant-specific tuning times and tuned FSM parameters are listed in Appendix Table IV. Trends in the tuned parameters included higher stiffness values during stance than in swing and highly-varying knee equilibrium angles across tasks. The observed gait was also noted to be quite sensitive to the tunable FSM transition criteria. Significant variance in the required tuning time for the different tasks was also observed.

2) *Steady-State Trials*: The kinematic and kinetic trajectories produced by the HKIC during the steady-state trials highlight its ability to reproduce normative biomechanics over variable tasks (Fig. 6). Bilinear interpolation was used to generate the able-bodied reference trajectories for tasks between those reported in the dataset [24]. The observed HKIC trajectories show strong similarity to the able-bodied references, particularly at the ankle. Knee moments are the most different relative to able-bodied for both the HKIC and the FSMC. The separation and trends seen in the HKIC closely resemble those observed the able-bodied data, suggesting appropriate adaptation in response to variable-task walking.

We quantified the similarity between the observed and able-bodied trajectories during stance and swing, showing that the HKIC produced a low RMSE in most metrics (Fig. 7). Stance and swing were treated separately to isolate the performance of the novel impedance parameter model (Section III), as it was only used during stance. The first 15 seconds at each task were neglected to allow time for the treadmill to reach steady-state. Unless otherwise specified, we present inter-participant averages and calculate standard deviations using lumped participant strides. Individual RMSE values for each participant were similar to the inter-participant averages and are available in the Appendix (Table V). The low RMSE values suggest that, in addition to replicating normative trends as task varied, the HKIC produced kinematics and kinetics that were close to the reference values. Further, the HKIC’s performance was as good as or better than the hand-tuned FSMC’s performance in seven of the eight metrics. The high knee kinematic error during swing can be attributed to the intentional early knee extension meant to improve user confidence (see Appendix Section A2) and it did not result in adverse gait effects.

Inter-participant spatiotemporal gait metrics also showed similarity to able-bodied data [24]. Both controllers elicited lower cadence gaits (equivalently longer stride length gaits)

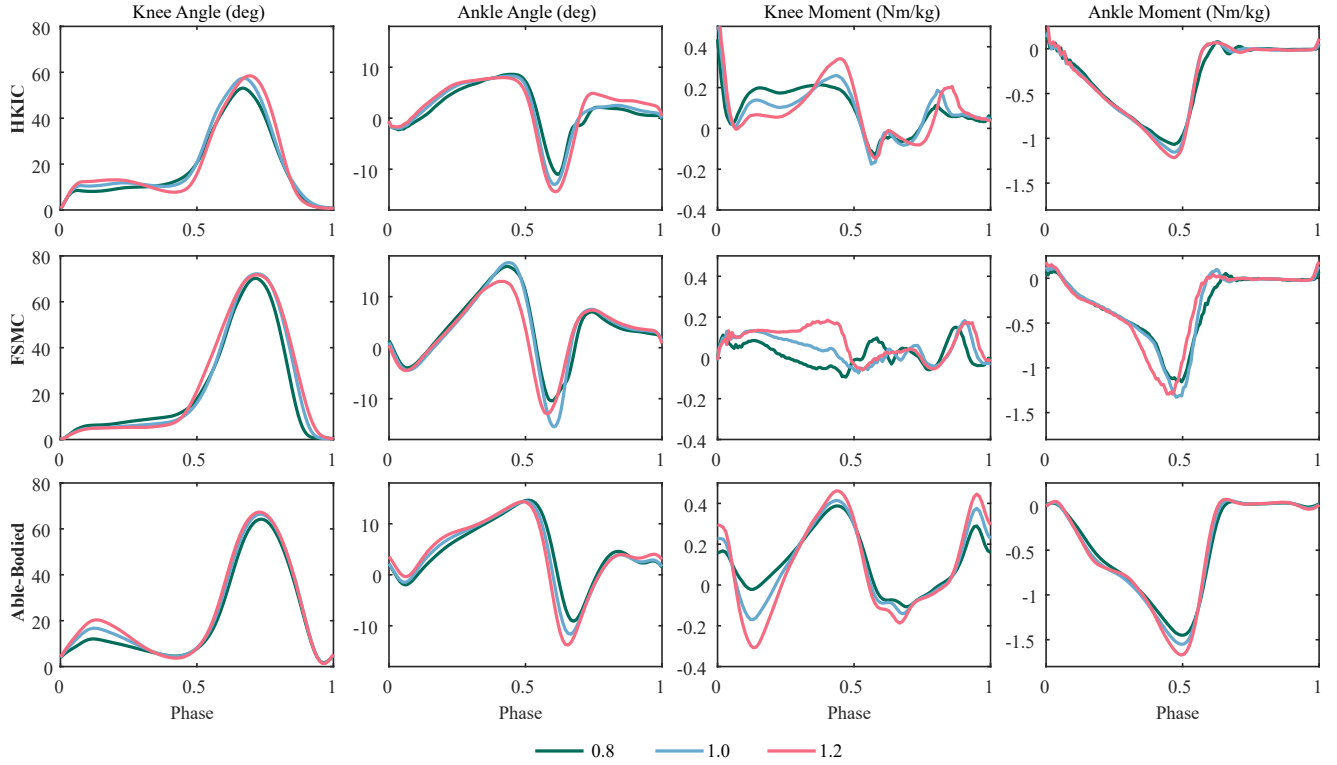
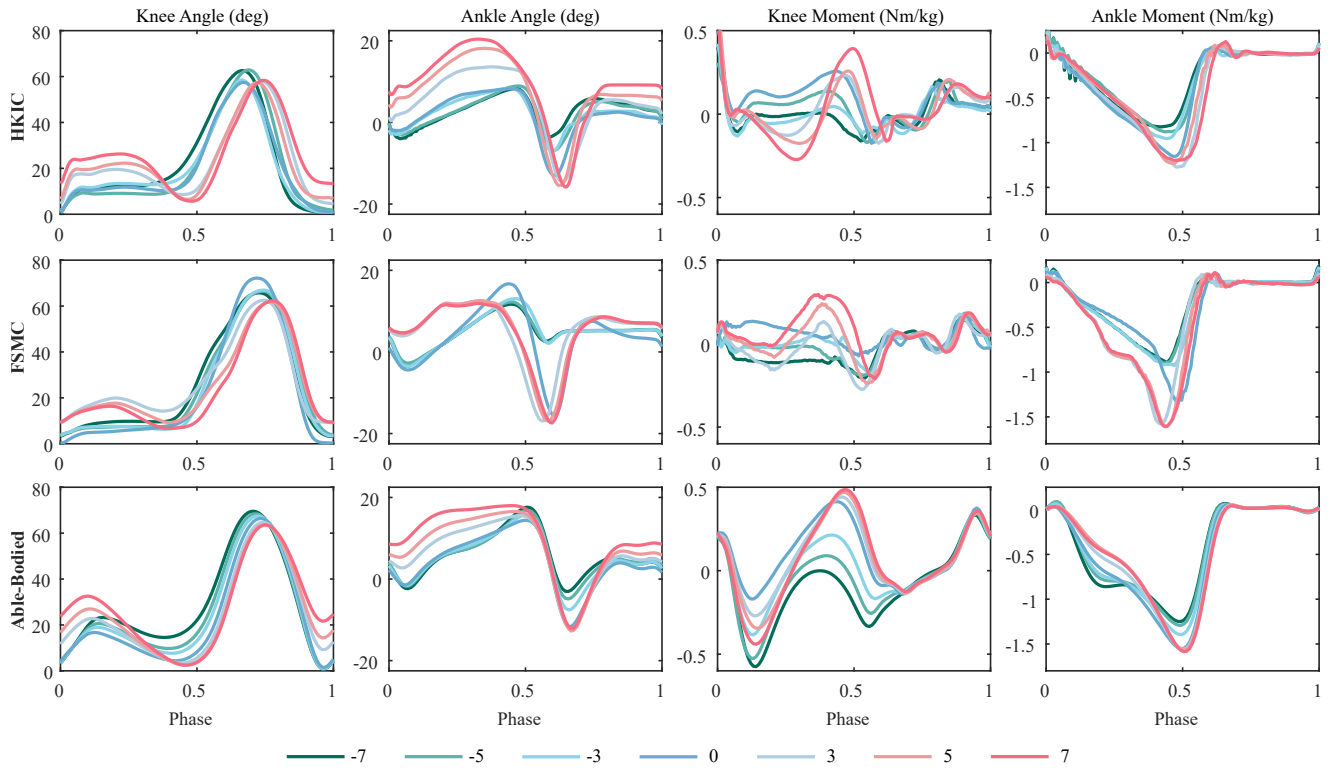


Fig. 6. Plots of the inter-participant average kinematic and kinetic trajectories produced by each controller over (a) varying inclines at 1 m/s and (b) varying speeds at level ground for the steady-state trials. Able-bodied trajectories from [24] are also shown for reference. The HKIC produced smooth kinematic variations with incline changes as well as increasing knee flexion and ankle push-off torque with increased speed, resembling the able-bodied trajectories.

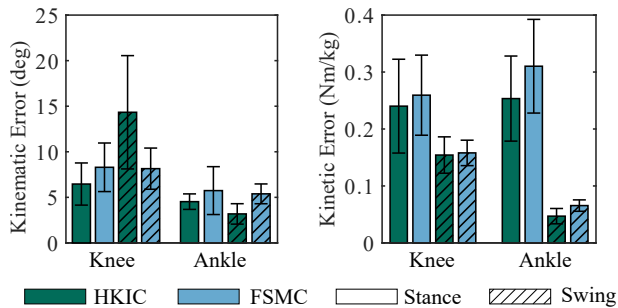


Fig. 7. Inter-participant RMSE in the observed kinematics (left) and kinetics (right) relative to able-bodied walking data for both the HKIC and FSMC during the steady-state task trials. The error bars represent ± 1 standard deviation over lumped participant strides. The HKIC demonstrated lower mean error than the FSMC in 7 of 8 metrics, with particular improvements at the ankle joint. The high knee kinematic error in swing for the HKIC is the result of intentional early extension to promote user confidence that the prosthesis was ready for weight acceptance.

compared to able-bodied, but show generally similar trends of increasing cadence with walking speed (Fig. 8). Additionally, the stance time symmetry ratio r_{STS} was calculated using the ground reaction force data, defined as the ratio between the average prosthetic stance time and the contralateral limb stance time. The mean and standard deviation over the steady-state trials of both participants were $r_{STS} = 0.902 \pm 0.017$ for the HKIC and $r_{STS} = 0.892 \pm 0.016$ for the FSMC. Note that due to a recording error, symmetry data was not available for participant P1’s HKIC SS-Decline trial. Both controllers produced a slightly more symmetric gait than average AKA participants with passive prostheses ($r_{STS} = 0.784$, reported in [64]), but less symmetric gaits than able-bodied people ($r_{STS} = 1.02$, reported in [65]).

The HKIC also produced trends in joint work across variable tasks that were consistent with able-bodied data (Fig. 9). As one of the benefits of impedance control is the ability to control energy exchange with the environment [10], the HKIC should be able to replicate this biological behavior. The HKIC showed similar trends as the able-bodied data, with a linear increase in net work performed with increasing incline, particularly at the ankle (increase of 0.0337 J/kg/deg , $R^2 = 0.982$). For comparison, able-bodied ankle work increases linearly at 0.0335 J/kg/deg with $R^2 = 0.987$. The HKIC also increased total work with increasing speed in a manner consistent with able-bodied data, though the work differences between the slow and fast speeds are minor for the able-bodied reference. In contrast, the net work performed by the FSMC decreased with speed and appeared discretized to three levels with respect to inclines, corresponding to its tuned tasks. Interestingly, the HKIC and FSMC showed less energy absorption at the knee during declines, which may reflect the habitual aversion to early stance knee flexion commonly observed in AKA populations [66], [67].

3) *Continuously-Varying Trials*: The continuously-varying trials demonstrated the HKIC’s ability to autonomously adapt behavior to the sensed walking speed and ground incline. The kinematic and kinetic errors were calculated in a similar manner for the continuously-varying task trials, though this

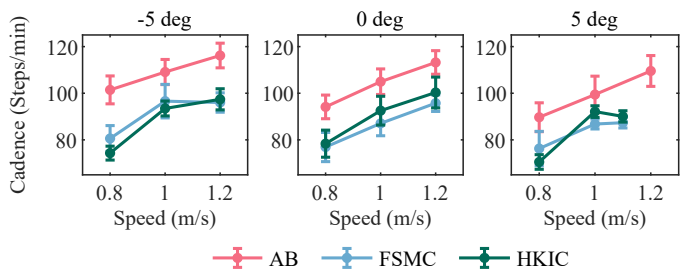


Fig. 8. Inter-participant average cadence for the steady-state task trials as functions of speed for different ramp inclinations: ramp descent (left), level ground (middle), and ramp ascent (right). Error bars represent ± 1 standard deviation over lumped participant strides. Both controllers show similar cadence trends as the able-bodied reference (AB) calculated from [24], with increasing step frequency with increasing speed. Overall, the participants preferred longer strides relative to able-bodied, which may be due to the larger mass of the powered prosthesis.

TABLE II
TASK ESTIMATE RMSE OBSERVED DURING THE CONTINUOUSLY-VARYING TASK TRIALS AVERAGED OVER LUMPED PARTICIPANT STRIDES

Trial	Controller	Incline (deg)	Speed (m/s)
CV-Incline	HKIC	0.61 ± 0.58	0.10 ± 0.07
	FSMC	1.81 ± 1.42	0.11 ± 0.06
CV-Decline	HKIC	0.66 ± 0.42	0.11 ± 0.07
	FSMC	1.03 ± 0.68	0.12 ± 0.07

time including strides that occurred during task transients. Fig. 10 shows the inter-participant average error trajectories at both joints for the CV-Incline trial, calculated as the able-bodied references subtracted from the observed values. Appendix Table V details the participant-specific stance and swing kinematic and kinetic RMSE for both the CV-Incline and CV-Decline trials. Aside from the late-swing knee kinematics (discussed above), the HKIC shows low errors throughout the gait cycle, particularly at the ankle joint. Further, the magnitude of the FSMC’s error is larger than the HKIC’s for most of the gait cycle, highlighting the importance of the HKIC’s continuously-adaptive nature.

As both controllers received no external task input during these trials, the task estimates (and the phase estimate for the HKIC) contributed to the kinematic and kinetic errors. The task estimate RMSE, averaged over each stride and participant, is shown in Table II for each trial. Although the same task estimation algorithms were used with both controllers, FSMC showed higher incline estimate error, suggesting that differences in controller behavior may have impacted the incline estimate’s efficacy. Additionally, the average phase estimate trajectories produced by HKIC during the CV-Incline and CV-Decline trials were highly linear (mean $R^2 = 0.989$) and accurate (mean RMSE of 6.157%), even as speed and incline varied (Fig. 11). However, the phase estimate saturated more often for participant P2 than participant P1, suggesting that participant P2’s high trajectory was less similar to able-bodied trajectories than participant P1’s.

VI. DISCUSSION

A. HKIC Performance

This work presented a data-driven, phase-based walking controller for a powered knee-ankle prosthesis that au-

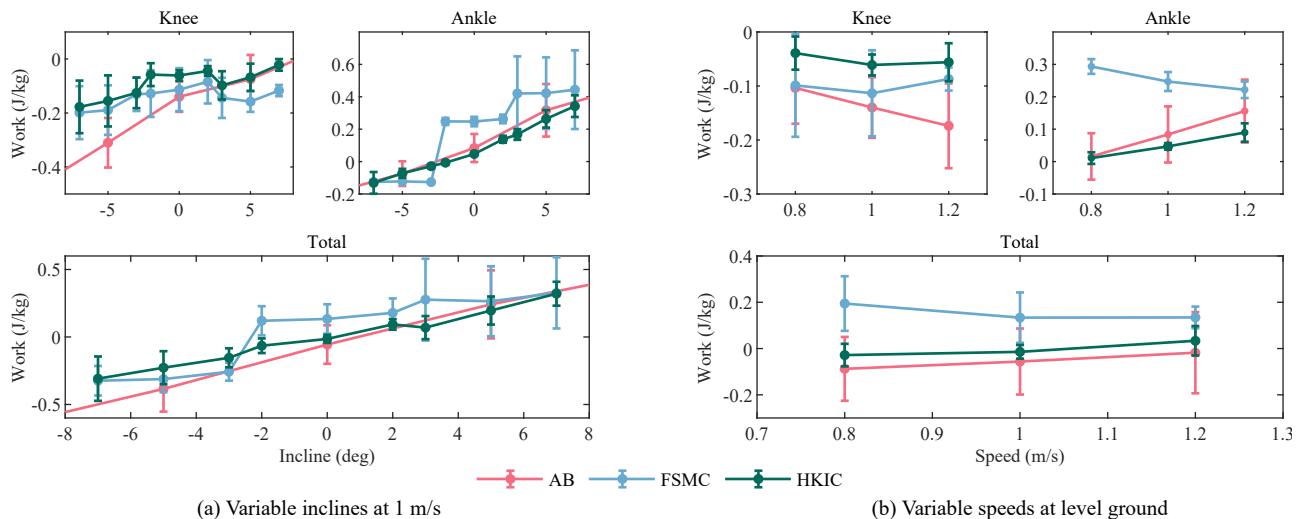


Fig. 9. The inter-participant average prosthesis work per stride over variable (a) inclines and (b) speeds during the steady-state task trials. Error bars represent ± 1 standard deviation over lumped participant strides. An able-bodied reference (AB) calculated from [24] shows that the HKIC demonstrated biomimetic energy injection, particularly through a linear increase in ankle work as incline increased, corresponding to 100.6% of the able-bodied rate. Both controllers showed less energy absorption at the knee during steep declines, suggesting that our participants may have had habitual aversions to early stance knee flexion.

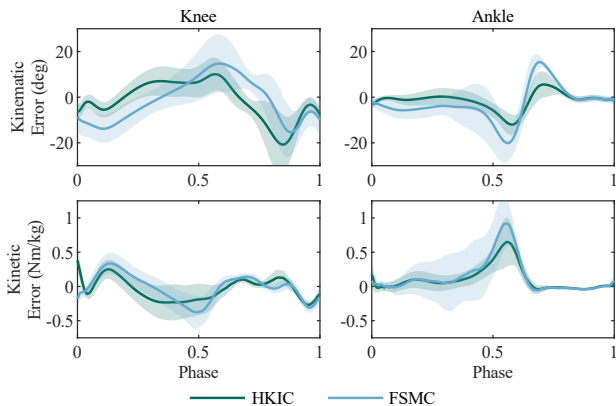


Fig. 10. Plot of the inter-participant average kinematic and kinetic error trajectories in the continuously-varying incline trial, relative to able-bodied data [24]. The knee data is shown in the left column and the ankle in the right. Shaded regions represent ± 1 standard deviation over lumped participant strides. Aside from intentional discrepancies in the late-swing knee kinematics (see Appendix Section A2), the HKIC showed low RMSE across the gait cycle throughout varying tasks, suggesting appropriately adapting biomechanics.

tonomously adapted its behavior across a continuous range of walking speeds and inclines. To achieve this without manual impedance tuning, we used an able-bodied dataset to optimize for continuous stiffness, damping, and equilibrium angle functions that reproduced biological stance joint torques, given biological kinematics. In an initial offline analysis, we showed that our optimized impedance parameter model produced joint torques with across-task average normalized RMSE values of 0.78 and 0.58 for the knee and ankle, respectively. The low normalized RMSE suggests that the model captures the essential joint dynamics of able-bodied walking.

The subsequent experiments with two AKA participants demonstrated that the identified impedance parameter functions also rendered appropriate stance phase joint mechanics when used for real-time control in the HKIC. Other normative walking features were observed, such as increasing ankle work with increasing incline (Fig. 9) and increasing cadence with

walking speed (Fig. 8). Although the kinematic and kinetic profiles produced by the HKIC had small differences relative to able-bodied data (Figs. 6-7), the participants exhibited qualitatively normal gait patterns over a wide array of tasks (see Supplemental Video). Kinematic and kinetic trends emerged with variable speeds and inclines that were consistent with able-bodied data (Fig. 6), including appropriately varying peak ankle moments, stance ankle kinematics, and knee stance kinematics. Knee swing kinematics showed the highest error for the HKIC, which was expected because we intentionally allowed the phase variable to saturate early to ensure full knee extension prior to heelstrike. Pilot testing showed that consistent full knee extension helped eliminate participants' problematic instinctive compensations and promoted confidence that the prosthesis was ready to accept weight (see Section A2). Small phase shifts result in large swing kinematic errors due to the large knee range of motion, and although the error values appear large, they did not interfere with the participants' gait or cause toe-stubbing.

Appropriate kinematic and kinetic adaptation are both practically and clinically important for the user. For example, knee swing kinematic adaptations enable the prosthesis to have the proper configuration at heelstrike as incline varies. Without such adaptations, the user may, for example, toe-stub during swing when walking uphill with level ground kinematics, or vice versa, experience too much flexion to enable heelstrike at the desired time. Further, kinetic adaptation during stance enables increasing peak ankle moments for propulsion as incline and speed increase (Fig. 6). Improper joint kinetics can cause improper ground reaction forces, which can affect user balance [68]. Finally, appropriate kinematic and kinetic co-adaptation enables joint work adaptation, even in cases where both kinematics and kinetics deviate from able-bodied normative trajectories. For example, the HKIC's peak ankle moment at a 7 deg incline is slightly smaller than able-bodied (Fig. 6). However, a corresponding increase in peak

plantarflexion angle allows the HKIC to maintain appropriate ankle work (Fig. 9). Biomimetic energy injection is important to prevent compensations from other joints and additional health problems [3]–[5], [41].

Qualitative remarks by the participants also testified to the biomimetic task adaptation of the HKIC. Participant P1 remarked while walking at the seven deg incline that he did not feel like he was walking uphill, suggesting appropriate joint dynamics and energy exchange. Participant P2 remarked that he did not even notice that the treadmill had transitioned to the 2 deg decline and that he could “climb up much easier” while ascending steep inclines. These anecdotal remarks further support the claim that the HKIC adapts to changing tasks to produce normative able-bodied biomechanics, which could result in many practical benefits for the user. For example, the biomimetic energy injection at steep inclines (Fig. 9) may allow users to walk uphill for longer before fatiguing.

While the FSMC’s performance was not drastically worse than the HKIC’s in the tested metrics, it required on average 10 minutes of tuning per tuned task. Although only 3 tasks were tuned for this study, practical deployment of the FSMC would likely require many more tasks to be tuned. For example, participant P2 noted that the FSMC was “kicking off way too hard” when going uphill at slow speeds, but was happy with its behavior at normal speeds, suggesting that more speed-specific impedance parameter sets could be beneficial. However, adding more tuning points is likely impractical in a clinical setting, especially without specialized equipment such as a variable-incline treadmill. Therefore, the HKIC’s potential to produce biomimetic behavior over varying tasks without manual impedance tuning is a significant benefit.

For online implementation of the continuous impedance parameter model, gait phase needed to be estimated in real-time. The improved phase variable behavior observed in simulation in Section IV-A was confirmed in the participant experiments. Fig. 11 shows how the phase variable eliminated the previously observed phase pause near push-off. The result of this monotonicity is visible in the kinematics of Fig. 6, as there is not a pause in the kinematic trajectories near push-off, which was observed previously in [49]. Further, the general linearity of the average phase trajectories in Fig. 11 (mean $R^2 = 0.989$) is improved compared to [49]. Because both the impedance and kinematic models in HKIC assume a perfectly linear phase estimate, the observed linearity keeps the model outputs of the controller synchronized with the user’s gait. Additionally, Fig. 11 shows that participant P2’s phase variable saturates at 1 earlier in the gait cycle than participant P1. This occurs because the methods used to estimate the thigh trajectory features (Appendix Section A2) prioritize phase saturation (and subsequently full knee extension) to promote participant confidence. This early phase saturation suggests that P2 preferred for the knee to be fully extended earlier in swing, whereas P1 was satisfied with full knee extension occurring right before heelstrike, as it does in able-bodied data.

The task estimates are other critical components required for walking over continuously-varying tasks. Seen in Table II, the error in the speed estimate was fairly consistent over the trials, with RMSE between 0.10 and 0.12 m/s for both

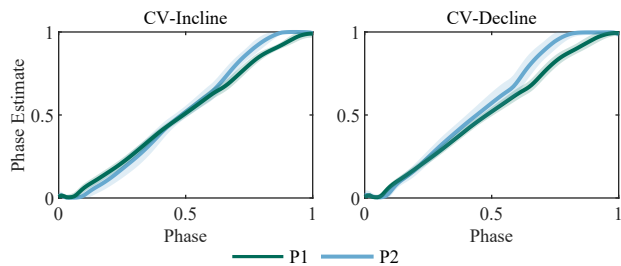


Fig. 11. Average phase estimate progression calculated in real-time by the HKIC during the continuously-varying task trials for participants P1 and P2. Shaded regions represent ± 1 standard deviation. The linearity and consistency of the trajectories illustrate the phase variable’s ability to adapt to continuous task variations and appropriately parameterize the gait cycle.

controllers. This error is likely due to a slightly asymmetric gait, which violates the assumptions made in the speed estimator’s formulation. Gait asymmetries may be the result of our participants’ habitual compensations, socket comfort, or the significant mass difference between the robotic prosthesis and participants’ passive prostheses. Interestingly, the incline estimate produced lower error with the HKIC (0.61 to 0.66 deg) than the FSMC (1.03 to 1.81 deg). We speculate that the higher error in the FSMC is due to a feedback interaction between incline estimate errors and the impedance parameters. Due to the discrete switching behavior of the impedance parameters (see Appendix Fig. 15b), a small incline estimate error can result in large changes in prosthesis behavior and may affect the θ_f and ℓ_{cop} progressions. Therefore, the continuous nature of the HKIC may be preferable, as it does not display discrete changes in behavior with small changes in task inputs.

B. Limitations and Future Work

The HKIC and this study were not without limitations. Our experiment provided a somewhat limited view of the HKIC’s behavior, as it involved only two participants, each with only one experimental session (although both had prior experience walking with the prosthesis). We expect that the data-driven impedance parameter model identified in Section III will yield similar performance for a wide array of participants, as it was created without *a priori* knowledge of the participants or their preferences. Preliminary studies of able-bodied users testing the HKIC over varying tasks suggest that this assumption holds [69]. However, this assumption should be validated in future studies with wider AKA participant pools, as the HKIC’s ability to generalize to the full AKA population remains unknown. Further, the performance of the HKIC should also be investigated when implemented on different hardware platforms to better validate the framework. While the HKIC could in theory be implemented on any powered prosthetic leg with the ability to render a variable joint impedance, prostheses with non-trivial actuator transmissions (*e.g.*, [6], [48]) or series elasticity (*e.g.*, [21], [61]) would require actuator characterization [70] and, in some cases, closed-loop torque control to accurately render variable joint impedance.

Additionally, it is possible that there are users for which the population average impedance parameters are not optimal. There may also exist other impedance parameter functions

that produce normative biomechanics, as the human sensorimotor system is highly adaptable [71]–[73]. Participants’ sensitivity to changes in the impedance parameter model could be investigated in future studies. Additionally, there may be factors other than those considered in this work that distinguish the ideal parameter functions, such as user preference. A study investigating users’ preferred stiffness in ankle prostheses showed that the preferred joint stiffness varies by user [74], which is likely true for AKA participants as well. For example, participant P2 noted that the knee felt “squishy” when ascending steep slopes and that he would have preferred it to be stiffer. While one of the major advantages of HKIC is that it required no manual impedance parameter tuning, it is currently limited by the lack of an ability to customize to an individual’s preferred behavior. Future work will investigate methods to incorporate user preferences in the impedance model, such as weighting the optimization with a single baseline personalization for level-ground walking, as suggested in [75]. This baseline personalization could be gathered using tools in a standard clinic [51], maintaining the minimal-tuning nature of the controller.

Our study also did not investigate discrete changes in ground slope, which may be encountered during daily ambulation (e.g., wheelchair ramps) and should be handled by a variable-task walking controller. While [49] showed that the HKIC’s incline estimation algorithm is stable under discrete incline changes, our task estimation methods are limited by their discrete “once-per-step” update nature. Because we detect incline during midstance, the user must, at a minimum, be able to complete the first half of stance phase with the previous stride’s task estimate. This is particularly problematic during discrete transitions between steep inclines and level ground walking because the heelstrike kinematics vary drastically [24]. Future work involving anticipatory algorithms that update the task estimate based on sensed characteristics of the upcoming terrain [76]–[78] or user behavior [79], [80] may be necessary to alleviate this limitation.

Further, this work only investigated rhythmic walking over relatively long durations, though almost half of all walking bouts in community ambulation contain less than 12 consecutive steps [81]. One of the unique strengths of the presented phase variable is the ability to intuitively control non-rhythmic tasks [31]. Although this capability of the HKIC was demonstrated at the beginning and end of each trial in this study, it should be explored further and characterized in future studies involving rapid start/stop, lateral movements, and other behaviors that are prominent in agile locomotion. Such studies may also highlight the limitations of using the current impedance parameter model for non-rhythmic tasks. Although the participants were able to achieve start/stop behaviors in this experiment, additional able-bodied data may need to be included in the optimization to produce appropriate impedance parameters for other non-rhythmic tasks.

The continuously-adaptive nature of the HKIC may also be a limitation in some circumstances. For example, participant P2 noted that while he appreciated that the HKIC always adapted to the current task, he also preferred the predictability of the FSMC. We plan to investigate methods to preserve the

flexibility of the HKIC while increasing predictability in future studies. One way to improve the predictability of the HKIC may be to increase the training duration to allow the participants to better acclimate to and leverage the benefits the HKIC and the powered prosthesis. Perhaps the lack of early stance knee flexion in both controllers (Fig. 10) and the low knee energy dissipation (Fig. 9) are less due to controller behavior and more due to the participant’s habitual compensations developed through years of using a passive prosthesis [66], [67]. Future work may show that as the participants become more comfortable with a powered prosthesis and develop a stronger intuition for the HKIC’s behavior, these gait features become more similar to able-bodied data.

Finally, there is much interesting work to be done investigating the relationship between biological joint impedance measured in empirical studies [12]–[14] and the impedance parameters used in impedance controllers. Mechanical impedance can only be characterized through perturbation studies, so the impedance parameters found by optimizing over non-perturbed gait data will not necessarily reflect these dynamics. We plan to study the effects of constraining the optimization with known empirical impedance values, as well as to investigate the HKIC’s behavior during gait perturbations.

VII. CONCLUSION

This work presented a data-driven walking controller designed to work over a continuum of speeds and inclines. We developed continuous models of joint stiffness, damping, and equilibrium angle for an impedance controller using convex optimization. We also presented an improved phase estimation algorithm, showing increased monotonicity and linearity. Two AKA prosthesis users demonstrated the controller’s ability to autonomously produce biomimetic behavior over continuously-varying tasks during treadmill experiments. The experiments showed that, when compared with able-bodied data, the presented controller produced biomimetic trends in joint kinematics, kinetics, work, and cadence, indicating its ability to render appropriate joint mechanics as task varied.

APPENDIX

A. Task-Invariant Phase Variable Algorithm

The new phase variable \hat{s} is calculated through a series of linear equations with θ_{th} as an input. An FSM controls when each equation is used. Although the FSM contains discrete states, the structure of the linear equations ensures that \hat{s} is continuous. Each equation is defined by quantitative features of the θ_{th} trajectory, which are measured in real-time. Table III lists the features’ definitions and notations. First, we give the rationale for each FSM state and its corresponding phase variable equation. Then, we present methods to estimate the thigh trajectory features in real-time, as well as the steps taken to promote closed-loop stability of the phase estimate.

1) *Phase Variable FSM*: Consider the average θ_{th} trajectory for an able-bodied individual walking at 1 m/s on level ground, shown in Fig. 12. The pertinent θ_{th} trajectory features used in the phase estimate are labeled, as well as the standard timing

of the FSM states. The overall structure of the FSM used to control the phase estimate is shown in Fig. 13.

The FSM begins in S1, occurring just after a heelstrike (HS) event. During S1, θ_{th} is linearly scaled as the hip joint extends from θ_{th}^{HS} to θ_{th}^{MHE} such that \hat{s} increases and $\hat{s} = s_{MHE}$ when $\theta_{th} = \theta_{th}^{MHE}$. Mathematically, this is given by

$$\hat{s} = \frac{\theta_{th}^{HS} - \theta_{th}}{\theta_{th}^{HS} - \theta_{th}^{MHE}} s_{MHE} \quad \text{in S1, S2.} \quad (22)$$

The FSM transitions to S2 at a phase estimate threshold $\hat{s}_{1 \rightarrow 2} = 0.1$, which typically corresponds to the point in the gait cycle where the θ_{th} trajectory becomes linear.

In S2, \hat{s} is calculated using the same linear relationship as in S1 (22), but is denoted as a distinct state because it represents a portion of the gait cycle where θ_{th} (and therefore \hat{s}) has constant velocity. The average rate of change of \hat{s} during S2 (\hat{s}_{S2}) is recorded for use in S3. The FSM transitions to S3 once $\hat{s}_{2 \rightarrow 3} = 0.9s_{MHE}$, which typically corresponds to the end of the linear portion of the thigh trajectory, or if $\dot{\theta}_{th} > 0$. This second case rarely occurs during steady walking, but is an important path to S3 in the event of an unusually short stride.

S3 occurs during the section of the gait cycle where θ_{th} reaches its minimum, and thus has a period of low angular velocity $\dot{\theta}_{th}$. Previous work has shown that sections of low $\dot{\theta}_{th}$ are problematic because they cause a pause in the phase variable trajectory [31], [41], [49]. This pause violates the assumption that \hat{s} increases monotonically and at a constant rate, resulting in incorrect kinematic and impedance model outputs. Therefore, during S3, we decouple \hat{s} from θ_{th} and instead assume that phase continues progressing at \hat{s}_{S2} :

$$\hat{s} = \hat{s}_{23} + \int_0^{\Delta t} \hat{s}_{S2} d\tau \quad \text{in S3.} \quad (23)$$

This feedforward phase progression continues until a toe-off (TO) event. Although this approach limits the user's ability to stop phase progression during S3, such cases are unlikely because stopping would inhibit power delivery from the ankle during push-off. Moreover, the under-actuated dynamics of bipedal walking dictate that once the user's gravity vector passes anterior of the stance foot, the user must continue the gait cycle until the contralateral foot lands [68], [82]. Therefore, we expect the sacrifice in direct control of phase progression during this section of the gait cycle to be negligible.

After TO, the FSM transitions to S4, where phase is again estimated via a linear scaling of θ_{th} . This mapping is defined such that \hat{s} increases from \hat{s}_{TO} towards s_{MHF} as θ_{th} increases:

$$\hat{s} = \frac{\theta_{th} - \theta_{th}^{TO}}{\theta_{th}^{MHF} - \theta_{th}^{TO}} (s_{MHF} - \hat{s}_{TO}) + \hat{s}_{TO} \quad \text{in S4.} \quad (24)$$

The FSM transitions to S5 when θ_{th} is equivalent to the average of θ_{th}^{HS} and θ_{th}^{MHF} , which typically corresponds to the end of this linear section of the thigh trajectory.

Two problems typically occurred with the previous phase variable methods when $\theta_{th} \approx \theta_{th}^{MHF}$, which occurs during S5 in the new FSM. First, a pause in \hat{s} would occur as θ_{th} slowed and θ_{th} approached θ_{th}^{MHF} , similar to the effect seen in S3. Second, the previous methods assumed that $\theta_{th}^{MHF} = \theta_{th}^{HS}$. In cases

TABLE III
SYMBOL DEFINITIONS FOR FEATURES USED TO CALCULATE \hat{s}

θ_{th}^{HS}	θ_{th} at heelstrike
θ_{th}^{MHE}	θ_{th} at maximum hip extension
θ_{th}^{MHF}	θ_{th} at maximum hip flexion
θ_{th}^{TO}	θ_{th} at toe off
s_{MHE}	s at maximum hip extension
s_{MHF}	s at maximum hip flexion
\hat{s}_{TO}	\hat{s} at toe off
\hat{s}_{S2}	Average rate of change of \hat{s} during S2
\hat{s}_{S4}	Average rate of change of \hat{s} during S4
Δt	Time since state transition
t_{MHE}	Time at maximum hip extension
t_{MHF}	Time at maximum hip flexion
t_0	Time at heelstrike
t_f	Time at gait cycle completion

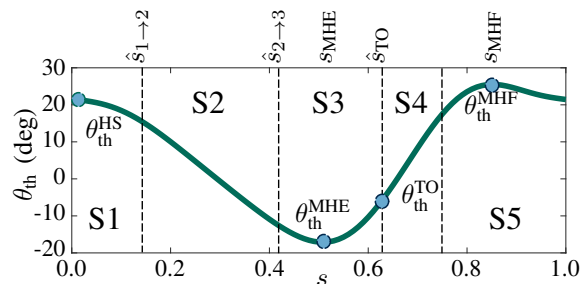


Fig. 12. The average global thigh angle trajectory θ_{th} (positive flexion) for 1 m/s 0 deg able-bodied walking, segmented by the phase variable FSM states. The phase variable is defined by linear mappings of θ_{th} during S1, S2 and S4, and by a feedforward phase variable rate during S3 and S5. The feedforward rates for S3 and S5 are given by the average rate of change of the phase estimates during the preceding states, which correspond to periods of constant thigh angular velocity.

where $\theta_{th}^{MHF} > \theta_{th}^{HS}$, such as the trajectory shown in Fig. 12, the resulting \hat{s} would saturate prematurely. Excessive saturation in the phase variable can cause desynchronization between the prosthesis and the user, leading to problems such as toe-stubbing. This effect was most exaggerated during declined walking, as the difference between θ_{th}^{MHF} and θ_{th}^{HS} was most pronounced [24]. To avoid both excessive saturation and a phase variable pause, a feedforward phase progression is again enforced based on the average phase rate in S4, \hat{s}_{S4} :

$$\hat{s} = \hat{s}_{45} + \int_0^{\Delta t} \hat{s}_{S4} d\tau \quad \text{in S5.} \quad (25)$$

This feedforward phase rate continues until either a heelstrike occurs or $\hat{s} = 1$. If the user is walking consistently and the θ_{th} trajectory feature estimates are correct, $\hat{s} = 1$ should occur simultaneously with heelstrike, returning the FSM to S1. If $\hat{s} = 1$ prior to HS, the FSM transitions to S6.

S6 is primarily encountered if the user pauses at the end of the gait cycle, so it does not appear in Fig. 12. During S6, \hat{s} is again calculated using a linear scaling of θ_{th} , giving the user volitional control of \hat{s} through θ_{th} :

$$\hat{s} = \frac{\theta_{th} - \theta_{th}^{MHE}}{\theta_{th}^{HS} - \theta_{th}^{MHE}} (1 - s_{MHE}) + s_{MHE} \quad \text{in S6.} \quad (26)$$

This volitional control during S6 is important because it allows movements such as kicking and non-steady leg swinging [31]. As in S5, a HS event returns the FSM to S1.

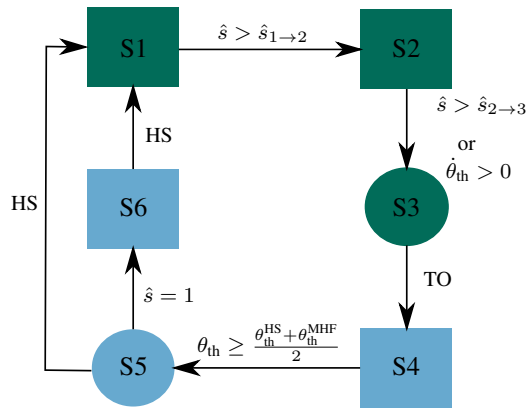


Fig. 13. Flow chart depicting the FSM states and transition criteria used in the phase variable calculation. States 1-3 (green) occur during the stance phase and states 4-6 (blue) occur during swing. States where phase is directly calculated based on thigh angle are shown as squares and states with feedforward definitions are shown as circles. State 6 is only necessary for non-steady gait and is typically bypassed during steady walking.

2) *Thigh Trajectory Feature Prediction:* The θ_{th} features used in (22)-(26) vary from stride-to-stride with changes in speed, incline, and natural gait variation. Some of these features are used in the phase estimate calculation before they occur in the gait cycle, specifically θ_{th}^{HS} , θ_{th}^{MHE} , θ_{th}^{MHF} , s_{MHE} and s_{MHF} . For example, θ_{th}^{MHE} is used to calculate \hat{s} during S1 and S2, but it does not typically occur until S3. Therefore, we predict these features in real-time based on observations from recent strides. At controller initialization, estimates of the thigh trajectory features are calculated using able-bodied data [24] and updated as new strides became available. Bounds were enforced on all estimated feature values to reject atypical strides and avoid stride-to-stride oscillation in the estimates.

Previous work showed that care must be exercised when predicting features of the thigh trajectory to prevent unwanted interaction between the prediction algorithms and the user's gait progression. For example, [49] observed that if a simple moving average was used to calculate θ_{th}^{MHE} , a divergent behavior occurred that resulted in the user taking progressively larger strides. To avoid this behavior, the kinematic features θ_{th}^{HS} , θ_{th}^{MHE} , and θ_{th}^{MHF} were estimated with moving average filters. These filters recorded the feature values from the previous 5 strides and averaged the median 3 for θ_{th}^{HS} and the minimum 3 for θ_{th}^{MHE} and θ_{th}^{MHF} . These filters were chosen to best reject non-representative strides, and the 5-stride window balanced between filter response time and variance rejection.

Another closed-loop interaction was observed during pilot studies regarding the predictions of s_{MHE} and s_{MHF} . In cases when the feature predictors were updating following a rapid change in task, we observed rare strides where \hat{s} underestimated the true phase at the end of the gait cycle, causing the knee joint to not fully extend before heelstrike. Participants instinctively responded by asymmetrically extending the late swing portion of the gait cycle to try force the knee to full extension. Moving average estimates of s_{MHE} and s_{MHF} , like those used for the kinematic features, caused s_{MHE} and s_{MHF} to decrease, resulting in further underestimation of \hat{s} on the subsequent stride. We suspect that participants behaved this

way because they were accustomed to passive prostheses, which will collapse upon loading if the knee is not fully extended. Therefore, new prediction methods were developed for s_{MHE} and s_{MHF} that favored \hat{s} saturation over underestimation to combat this instinctive behavior. Let $t_{\hat{s}=1}$ be the first time during the stride that $\hat{s} = 1$. Then, the s_{MHE} and s_{MHF} estimates were calculated as

$$s_{MHE} = \frac{1}{2} \left(\frac{t_{MHE} - t_0}{t_f - t_0} + \frac{t_{MHE} - t_0}{t_{\hat{s}=1} - t_0} \right), \quad (27)$$

$$s_{MHF} = \frac{1}{2} \left(\frac{t_{MHF} - t_0}{t_f - t_0} + \frac{t_{MHF} - t_0}{t_{\hat{s}=1} - t_0} \right).$$

The first quotient in each line of (27) is the true phase where θ_{th}^{MHE} and θ_{th}^{MHF} occurred. The second quotient is an upper bound on this true phase. We average the two so that \hat{s} favors saturation and full knee extension in late swing, avoiding the potential unstable feedback loop with the user's instinctive compensations. The results of (27) were likewise low-pass filtered with an infinite impulse response (IIR) filter to reject stride-to-stride variation and to prevent step estimate changes.

Finally, to calculate the stance phase \hat{s}_{st} , the expected value of \hat{s} at TO, \hat{s}_{TO} , must be estimated. This was calculated with a minimum moving average filter of \hat{s}_{TO} observed during previous strides, similar to the thigh trajectory features. The average window was 9 strides long, as the toe-off phase exhibits slow changes with task. Like the thigh trajectory features, \hat{s}_{TO} was initialized from able-bodied data.

Note that some minor aspects of the thigh trajectory feature estimation algorithms were modified after P1's experiment to better accommodate adaptation for users with thigh kinematics that differ significantly from able-bodied, such as P2. Namely, the feature estimate bounds were added, the θ_{th}^{MHE} and θ_{th}^{MHF} filters were changed from moving average to moving minimum filters, and the \hat{s}_{TO} filter was changed from an IIR filter to a moving minimum filter. A post-hoc simulation of P1's data before and after the minor adjustments showed only a 1.89% mean absolute difference in phase estimate between methods, suggesting that the changes would not have had an appreciable effect on his results. Further, no distinguishable effects were observed in the able-bodied simulation (Fig. 3c).

3) *Phase Variable Linearization:* The phase variable described above produces a consistent phase estimate trajectory over each stride during steady walking. This consistency allows a linearization map to be formed in order to further improve the phase estimate. Once the θ_{th} feature predictions converged to steady values, the average progression of \hat{s} was recorded for each steady walking stride and low-pass filtered to produce an average trajectory, $\bar{\hat{s}}$. The time constant of the IIR low-pass filter was chosen to be sufficiently slow (19 strides) such that the transients of the θ_{th} feature predictors were rejected. As a further precaution, any saturated portions of \hat{s} were discarded prior to averaging, as they diminish as the θ_{th} trajectory feature predictions converge.

The average phase was written as a function of true phase, given by $\bar{\hat{s}} = \sigma(s)$. Although the shape of the thigh trajectory may cause $\sigma(s)$ to be nonlinear, it is monotonic during normal walking. This implies that an inverse relationship $s = \sigma^{-1}(\bar{\hat{s}})$ exists, which can be applied to correct for nonlinearities in

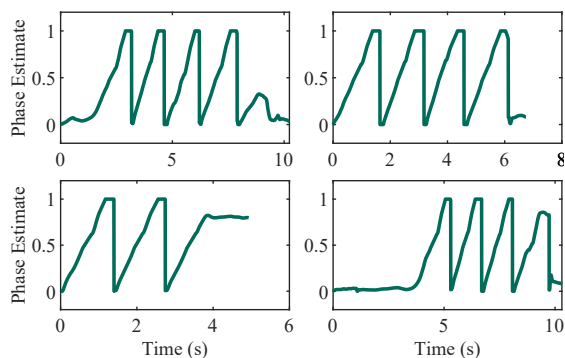


Fig. 14. Phase variable trajectories from 4 overground walking bouts recorded while Participant P1 acclimated to the prosthesis between parallel bars. The phase variable is able to parameterize these non-rhythmic motions, allowing the participant to start and stop the gait cycle at will.

\hat{s} . First, $\sigma(s)$ was fit with a 6th order polynomial $\bar{\sigma}(s)$ that was constrained with a minimum slope of 0.2. This minimum slope ensured strict monotonicity and numerical stability of the inverse. At each HS event, $\bar{\sigma}(s)$ was recalculated to incorporate the previous stride's effect on \hat{s} . Then the final, linearized phase estimate was calculated by applying the inverse map $\bar{\sigma}^{-1}$ to the results of (22)-(26).

4) *Phase Variable Results*: Fig. 11 highlights the new phase variable algorithm's ability to parameterize variable-incline walking, as consistent phase trajectories were produced for both participants during the continuously-varying task trials. The feedforward states S3 and S5 allowed for a positive phase rate, even when thigh velocity was low. Additionally, the thigh trajectory features were appropriately estimated, allowing a consistent phase estimates that were independent of the variable thigh trajectories seen with varying inclines. The phase linearization algorithm ensured highly linear estimates, with mean $R^2 = 0.997$ for participant P1 and mean $R^2 = 0.982$ for participant P2. Finally, the volitional start/stop behavior of the phase variable originally shown in [31] was preserved. Fig. 14 shows the phase variable trajectory for 4 non-steady bouts during the overground acclimation for participant P1, confirming its ability to parameterize non-rhythmic motion.

B. Benchmark FSM Impedance Controller

The Finite State Machine controller (FSMC), based on the FSM impedance controller presented in [16], was constructed to provide a benchmark with which to compare the HKIC. The flow of the FSMC's state machine is depicted in Figure 15. A tunable center of pressure threshold, ℓ_{cop}^* , controlled the transition from S1 to S2. Then, after a tunable duration, $t_{2 \rightarrow 3}$, the FSM transitioned to S3. Next, a TO event triggered the transition to S4. Finally, knee extension ($\dot{\theta}_k < 0$) caused a transition to S5, where the FSM remained until returning to S1 at HS. During transitions, the impedance parameters were rate-limited to prevent step changes in torque. In the FSMC, the torque command was given by (1), where K , B , and θ_{eq} depended on the current FSM state (given in Table IV).

Many methods have been proposed for deciding when to switch between sets of impedance parameters for different tasks, including simple threshold methods [16] and more

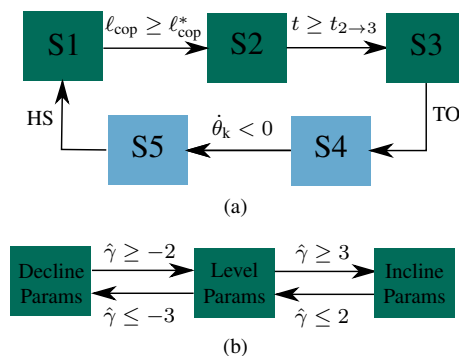


Fig. 15. (a) The structure and transition logic of the benchmark finite state machine controller. Tunable parameters ℓ_{cop}^* and $t_{2 \rightarrow 3}$ controlled the transitions from S1 to S2 and S2 to S3, while constant ground contact and knee velocity thresholds controlled the other three. States in green occur during stance and blue states during swing. (b) Task transition logic indicating how the impedance parameter sets are selected based on the incline estimate $\hat{\gamma}$.

complex machine learning methods [83], [84]. We employed a strategy similar to [16] where the prosthesis directly estimated the ground incline using the method described in Section IV-B. Then a secondary FSM was used to select between parameter sets based on the estimated incline $\hat{\gamma}$. To prevent rapid switching between parameters at the boundaries, overlap was included in the switching thresholds (Fig. 15b).

C. Additional Detailed Results

Table IV lists the results from the impedance parameter tuning for the FSMC, including the tuned impedance parameters, transition thresholds, and tuning times. The stiffness K , damping B , and equilibrium angle θ_{eq} were tuned by the research team for each of the 5 states (S1, S2, S3, S4, and S5) at three baseline tasks for each participant. Next, Table V shows the kinematic and kinetic RMSE values for each participant during both the steady-state and continuously varying trials, each separated by stance and swing.

ACKNOWLEDGEMENT

The authors thank Vamsi Peddinti for technical assistance with the robotic leg and Leslie Wontorcik, CP, for clinical support during experiments. We also thank Dr. Kyle Embry for prior contributions to the swing kinematic model.

REFERENCES

- [1] M. R. Tucker, J. Olivier, A. Pagel, H. Bleuler, M. Bouri, O. Lambercy, J. R. Del Millán, R. Riener, H. Vallery, and R. Gassert, "Control strategies for active lower extremity prosthetics and orthotics: A review," *J. Neuroeng. Rehabil.*, vol. 12, no. 1, 2015.
- [2] J. J. Genin, G. J. Bastien, B. Franck, C. Detrembleur, and P. A. Willems, "Effect of speed on the energy cost of walking in unilateral traumatic lower limb amputees," *Eur. J. of Appl. Physiol.*, vol. 103, 2008.
- [3] D. C. Norvell, J. M. Czerniecki, G. E. Reiber, C. Maynard, J. A. Pecoraro, and N. S. Weiss, "The prevalence of knee pain and symptomatic knee osteoarthritis among veteran traumatic amputees and nonamputees," *Arch. Phys. Med. Rehabil.*, vol. 86, no. 3, pp. 487–493, 2005.
- [4] P. A. Struyf, C. M. van Heugten, M. W. Hitters, and R. J. Smeets, "The Prevalence of Osteoarthritis of the Intact Hip and Knee Among Traumatic Leg Amputees," *Archives of Physical Medicine and Rehabilitation*, vol. 90, no. 3, pp. 440–6, 2009.

TABLE IV

RESULTS OF THE IMPEDANCE PARAMETER TUNING FOR THE FSMC FOR BOTH PARTICIPANTS P1 AND P2 AT EACH BASELINE TASK. THE FSMC CONSISTS OF 5 STATES: S1, S2, S3, S4, AND S5, EACH WITH UNIQUE PARAMETERS.

Participant P1		SS-Level - (0 deg, 1 m/s)					SS-Incline - (5 deg, 1 m/s)					SS-Divide - (-5 deg, 1 m/s)				
Tuning Time		3 min					14 min					5 min				
Transition		ℓ_{cop}^* 8.00 cm					5.00 cm					10.00 cm				
Parameters		$t_{2 \rightarrow 3}$ 0.091 s					0.190 s					0.061 s				
Impedance		S1	S2	S3	S4	S5	S1	S2	S3	S4	S5	S1	S2	S3	S4	S5
Knee	K (Nm/kg)	2.25	2.00	1.00	1.25	0.75	1.50	1.50	0.75	1.00	1.00	2.25	2.00	1.00	1.00	1.00
	B (Nms/kg)	0.14	0.13	0.12	0.07	0.06	0.09	0.09	0.09	0.08	0.07	0.09	0.10	0.10	0.05	0.07
	θ_{eq} (rad)	0.15	0.25	1.20	1.30	-0.15	0.35	0.25	0.50	1.20	0.30	0.15	0.35	0.75	1.25	0.05
Ankle	K (Nm/kg)	1.50	3.50	4.50	0.10	0.50	3.50	3.50	4.00	0.35	1.00	3.50	3.50	3.50	1.00	1.00
	B (Nms/kg)	0.14	0.14	0.14	0.13	0.10	0.14	0.14	0.14	0.15	0.10	0.10	0.10	0.10	0.10	0.10
	θ_{eq} (rad)	-0.10	-0.30	-0.35	0.20	0.00	0.10	-0.10	-0.23	0.20	0.10	0.100	-0.050	0.00	0.10	0.10

Participant P2		SS-Level - (0 deg, 1 m/s)					SS-Incline - (5 deg, 1 m/s)					SS-Divide - (-5 deg, 1 m/s)				
Tuning Time		19 min					16 min					4 min				
Transition		ℓ_{cop}^* 9.25 cm					7.25 cm					12.50 cm				
Parameters		$t_{2 \rightarrow 3}$ 0.090 s					0.230 s					0.061 s				
Impedance		S1	S2	S3	S4	S5	S1	S2	S3	S4	S5	S1	S2	S3	S4	S5
Knee	K (Nm/kg)	2.25	2.00	1.00	1.25	1.15	2.25	2.00	1.20	1.00	1.50	2.25	2.00	1.00	1.00	1.00
	B (Nms/kg)	0.14	0.13	0.12	0.06	0.07	0.09	0.09	0.09	0.08	0.09	0.14	0.13	0.12	0.08	0.05
	θ_{eq} (rad)	0.15	0.25	1.40	1.40	0.05	0.25	0.25	0.40	1.20	0.10	0.10	0.35	0.85	1.25	0.05
Ankle	K (Nm/kg)	1.50	3.00	4.00	0.10	0.50	2.50	2.00	4.00	1.00	1.00	1.00	3.50	4.50	1.00	1.00
	B (Nms/kg)	0.14	0.14	0.14	0.13	0.10	0.14	0.15	0.14	0.14	0.10	0.14	0.14	0.14	0.10	0.10
	θ_{eq} (rad)	-0.10	-0.30	-0.35	0.20	0.00	0.05	-0.10	-0.5	0.25	0.10	-0.05	-0.05	0.00	0.10	0.10

TABLE V

KINEMATIC AND KINETIC RMSE RELATIVE TO ABLE-BODIED DATA FOR THE KNEE (K) AND ANKLE (A) DURING THE STEADY-STATE AND CONTINUOUSLY VARYING TRIALS OF EACH PARTICIPANT

		Steady-State Trials								Continuously Varying Trials							
		Stance				Swing				Stance				Swing			
		Angle (deg)		Moment (Nm/kg)		Angle (deg)		Moment (Nm/kg)		Angle (deg)		Moment (Nm/kg)		Angle (deg)		Moment (Nm/kg)	
		K	A	K	A	K	A	K	A	K	A	K	A	K	A	K	A
P1	HKIC	5.08	4.93	0.22	0.30	9.70	2.51	0.14	0.04	4.71	5.06	0.20	0.27	7.28	2.64	0.13	0.04
	FSMC	8.07	6.78	0.23	0.37	7.86	5.69	0.16	0.06	8.15	7.38	0.21	0.39	7.90	5.86	0.16	0.06
P2	HKIC	7.83	4.09	0.26	0.20	17.98	3.83	0.17	0.06	8.10	3.75	0.28	0.19	16.81	3.67	0.16	0.06
	FSMC	8.42	4.92	0.28	0.25	8.62	5.19	0.16	0.07	8.30	5.76	0.24	0.27	9.35	5.09	0.15	0.06
AVG	HKIC	6.48	4.50	0.24	0.25	13.90	3.18	0.15	0.05	6.40	4.40	0.24	0.23	12.04	3.15	0.15	0.05
	FSMC	8.26	5.81	0.26	0.31	8.25	5.43	0.16	0.07	8.22	6.57	0.22	0.33	8.62	5.47	0.16	0.06

- [5] D. M. Ehde, D. G. Smith, J. M. Czerniecki, K. M. Campbell, D. M. Malchow, and L. R. Robinson, "Back pain as a secondary disability in persons with lower limb amputations," *Arch. Phys. Med. Rehabil.*, vol. 82, no. 6, pp. 731–734, 2001.
- [6] B. E. Lawson, J. Mitchell, D. Truex, A. Shultz, E. Ledoux, and M. Goldfarb, "A robotic leg prosthesis: Design, control, and implementation," *IEEE Robot. Autom. Mag.*, vol. 21, no. 4, pp. 70–81, 2014.
- [7] M. Windrich, M. Grimmer, O. Christ, S. Rinderknecht, and P. Beckerle, "Active lower limb prosthetics: A systematic review of design issues and solutions," *BioMed. Eng. Online*, vol. 15, 2016.
- [8] B. Laschowski, J. McPhee, and J. Andrysek, "Lower-limb prostheses and exoskeletons with energy regeneration: Mechatronic design and optimization review," *J. Mechanisms Robotics*, vol. 11, no. 4, 05 2019.
- [9] R. R. Torrealba and E. D. Fonseca-Rojas, "Toward the Development of Knee Prostheses: Review of Current Active Devices," *Appl. Mech. Rev.*, vol. 71, no. 3, pp. 1–22, 2019.
- [10] N. Hogan, "Impedance control: An approach to manipulation: Part i—theory," *J. Dyn. Syst. Meas. Control*, vol. 107, no. 1, pp. 1–7, 1985.
- [11] P. M. Rack and D. R. Westbury, "The short range stiffness of active mammalian muscle and its effect on mechanical properties," *J. Physiol.*, vol. 240, no. 2, 1974.
- [12] E. Rouse, L. Hargrove, E. Perreault, and T. Kuiken, "Estimation of human ankle impedance during the stance phase of walking," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 22, no. 4, pp. 870–878, 2014.
- [13] H. Lee and N. Hogan, "Time-varying ankle mechanical impedance during human locomotion," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 23, no. 5, pp. 755–764, 2015.
- [14] A. L. Shorter and E. J. Rouse, "Mechanical impedance of the ankle during the terminal stance phase of walking," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 26, no. 1, pp. 135–143, jan 2018.
- [15] F. Sup, H. Varol, J. Mitchell, T. Withrow, and M. Goldfarb, "Self-contained powered knee and ankle prosthesis: Initial evaluation on a transfemoral amputee," *IEEE Int. Conf. Rehabil. Robot.*, pp. 638–644, 2009.
- [16] F. Sup, H. A. Varol, and M. Goldfarb, "Upslope walking with a powered knee and ankle prosthesis: Initial results with an amputee subject," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 19, no. 1, pp. 71–78, 2011.
- [17] A. H. Shultz, J. E. Mitchell, D. Truex, B. E. Lawson, E. Ledoux, and M. Goldfarb, "A walking controller for a powered ankle prosthesis," *Conf. Proc. IEEE Eng. Med. Biol. Soc.*, pp. 6203–6206, 2014.
- [18] A. H. Shultz, B. E. Lawson, and M. Goldfarb, "Variable Cadence Walking and Ground Adaptive Standing with a Powered Ankle Prosthesis," *IEEE Trans. Neural Syst. Rehabilitation Eng.*, vol. 24, no. 4, pp. 495–505, 2016.
- [19] K. Bhakta, J. Camargo, P. Kunapuli, L. Childers, and A. Young, "Impedance control strategies for enhancing sloped and level walking capabilities for individuals with transfemoral amputation using a powered multi-joint prosthesis," *Mil. Med.*, vol. 185, pp. 490–499, 2020.
- [20] A. M. Simon, K. A. Ingraham, N. P. Fey, S. B. Finucane, R. D. Lipschutz, A. J. Young, and L. J. Hargrove, "Configuring a powered knee and ankle prosthesis for transfemoral amputees within five specific ambulation modes," *PLoS One*, vol. 9, no. 6, 2014.
- [21] E. J. Rouse, L. M. Mooney, and H. M. Herr, "Clutchable series-elastic actuator: Implications for prosthetic knee design," *Int. J. Rob. Res.*, vol. 33, no. 13, pp. 1611–1625, 2014.
- [22] G. Hunt, S. Hood, and T. Lenzi, "Stand-Up, Squat, Lunge, and Walk with a Robotic Knee and Ankle Prosthesis under Shared Neural Control," *IEEE Open J. Eng. Med. Biol.*, vol. 2, pp. 267–277, 2021.
- [23] K. Embry, D. J. Villarreal, R. L. Macaluso, and R. D. Gregg, "Modeling the Kinematics of Human Locomotion over Continuously Varying

- Speeds and Inclines," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 26, no. 12, pp. 2342–2350, 2018.
- [24] E. Reznick, K. R. Embry, R. Neuman, E. Bolívar-Nieto, N. P. Fey, and R. D. Gregg, "Lower-limb kinematics and kinetics during continuously varying human locomotion," *Sci. Data*, vol. 8, 2021.
- [25] A. Mohammadi and R. D. Gregg, "Variable Impedance Control of Powered Knee Prostheses Using Human-Inspired Algebraic Curves," *J. Comput. Nonlinear Dyn.*, vol. 14, no. 10, pp. 1–10, 2019.
- [26] W. Hong, V. Paredes, K. Chao, S. Patrick, and P. Hur, "Consolidated control framework to control a powered transfemoral prosthesis over inclined terrain conditions," *IEEE Int. Conf. Robot. Autom.*, pp. 2838–2844, 2019.
- [27] N. A. Kumar, W. Hong, and P. Hur, "Impedance control of a transfemoral prosthesis using continuously varying ankle impedances and multiple equilibria," *IEEE Int. Conf. Robot. Autom.*, pp. 1755–1761, 2020.
- [28] N. Anil Kumar, S. Patrick, W. Hong, and P. Hur, "Control framework for sloped walking with a powered transfemoral prosthesis," *Front. Neurobot.*, vol. 15, no. Jan, pp. 1–12, 2022.
- [29] F. J. Abu-Dakka and M. Saveriano, "Variable impedance control and learning—a review," *Front. Robot. AI*, vol. 7, 2020.
- [30] N. Hogan, "Adaptive control of mechanical impedance by coactivation of antagonist muscles," *IEEE Trans. on Automat. Contr.*, vol. 29, pp. 681–690, 1984.
- [31] S. Rezaeadeh, D. Quintero, N. Divekar, E. Reznick, L. Gray, and R. D. Gregg, "A phase variable approach for improved rhythmic and non-rhythmic control of a powered knee-ankle prosthesis," *IEEE Access*, vol. 7, pp. 109 840–109 855, 2019.
- [32] S. Boyd and L. Vandenberghe, *Convex Optimization*. Cambridge University Press, 2004.
- [33] T. Lenzi, L. Hargrove, and J. Sensinger, "Speed-adaptation mechanism: Robotic prostheses can actively regulate joint torque," *IEEE Robot. Autom. Mag.*, vol. 21, no. 4, pp. 94–107, 2014.
- [34] B. E. Lawson, B. Ruhe, A. Shultz, and M. Goldfarb, "A Powered Prosthetic Intervention for Bilateral Transfemoral Amputees," *IEEE Trans. Biomed. Eng.*, vol. 62, no. 4, pp. 1042–1050, 2015.
- [35] E. D. Ledoux and M. Goldfarb, "Control and evaluation of a powered transfemoral prosthesis for stair ascent," *IEEE Trans. Neural Syst. Rehabilitation Eng.*, vol. 25, 2017.
- [36] K. J. Kaveny, A. M. Simon, T. Lenzi, S. B. Finucane, E. A. Seyforth, G. Finco, K. L. Culler, and L. J. Hargrove, "Initial Results of a Variable Speed Knee Controller for Walking with a Powered Knee and Ankle Prosthesis," *Proc. IEEE RAS EMBS Int. Conf. Biomed. Robot. Biomechatronics*, vol. 2018-Augus, pp. 764–769, 2018.
- [37] T. Lenzi, M. Cempini, L. Hargrove, and T. Kuiken, "Design, development, and testing of a lightweight hybrid robotic knee prosthesis," *Int. J. Rob. Res.*, vol. 37, no. 8, pp. 953–976, 2018.
- [38] J. Mendez, S. Hood, A. Gunnell, and T. Lenzi, "Powered knee and ankle prosthesis with indirect volitional swing control enables level-ground walking and crossing over obstacles," *Sci. Robot.*, vol. 5, no. 44, 2020.
- [39] T. Elery, S. Rezaeadeh, C. Nesler, and R. D. Gregg, "Design and validation of a powered knee-ankle prosthesis with high-torque, low-impedance actuators," *IEEE Trans. Robot.*, vol. 36, no. 6, pp. 1649–1668, 2020.
- [40] S. Hood, L. Gabert, and T. Lenzi, "Powered Knee and Ankle Prosthesis With Adaptive Control Enables Climbing Stairs With Different Stair Heights, Cadences, and Gait Patterns," *IEEE Trans. Robot.*, vol. 38, no. 3, pp. 1430–1441, 2022.
- [41] T. Elery, S. Rezaeadeh, E. Reznick, L. Gray, and R. D. Gregg, "Effects of a Powered Knee-Ankle Prosthesis on Amputee Hip Compensations: A Case Series," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 28, no. 12, pp. 2944–2954, 2020.
- [42] L. Gabert, S. Hood, M. Tran, M. Cempini, and T. Lenzi, "A compact, lightweight robotic ankle-foot prosthesis: Featuring a powered polycentric design," *IEEE Robot. Autom. Mag.*, vol. 27, no. 1, pp. 87–102, mar 2020.
- [43] H. L. Bartlett, S. T. King, M. Goldfarb, and B. E. Lawson, "A Semi-Powered Ankle Prosthesis and Unified Controller for Level and Sloped Walking," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 29, pp. 320–329, 2021.
- [44] H. Huang, D. L. Crouch, M. Liu, G. S. Sawicki, and D. Wang, "A Cyber Expert System for Auto-Tuning Powered Prosthesis Impedance Control Parameters," *Ann. Biomed. Eng.*, vol. 44, no. 5, pp. 1613–1624, 2016.
- [45] M. Li, Y. Wen, X. Gao, J. Si, and H. Huang, "Toward expedited impedance tuning of a robotic prosthesis for personalized gait assistance by reinforcement learning control," *IEEE Trans. Robotics*, vol. 38, no. 1, pp. 407–420, 2022.
- [46] R. Wu, M. Li, Z. Yao, W. Liu, J. Si, and H. Huang, "Reinforcement learning impedance control of a robotic prosthesis to coordinate with human intact knee motion," *IEEE Robotics and Automation Letters*, vol. 7, no. 3, pp. 7014–7020, 2022.
- [47] R. D. Gregg, T. Lenzi, L. J. Hargrove, and J. W. Sensinger, "Virtual constraint control of a powered prosthetic leg: From simulation to experiments with transfemoral amputees," *IEEE Trans. Robot.*, vol. 30, no. 6, pp. 1455–1471, 2014.
- [48] D. Quintero, D. J. Villarreal, D. J. Lambert, S. Kapp, and R. D. Gregg, "Continuous-Phase Control of a Powered Knee-Ankle Prosthesis: Amputee Experiments Across Speeds and Inclines," *IEEE Trans. Robot.*, vol. 34, no. 3, pp. 686–701, 2018.
- [49] T. K. Best, K. Embry, E. J. Rouse, and R. D. Gregg, "Phase-variable control of a powered knee-ankle prosthesis over continuously varying speeds and inclines," *IEEE Int. Conf. Intelli. Robot. Sys.*, 2021.
- [50] R. J. Cortino, E. Bolivar-Nieto, T. K. Best, and R. D. Gregg, "Stair ascent phase-variable control of a powered knee-ankle prosthesis," in *IEEE Int. Conf. Robot. Autom.*, 2022, pp. 5673–5678.
- [51] D. Quintero, E. Reznick, D. J. Lambert, S. Rezaeadeh, L. Gray, and R. D. Gregg, "Intuitive Clinician Control Interface for a Powered Knee-Ankle Prosthesis: A Case Study," *IEEE J. Transl. Eng. Heal. Med.*, vol. 6, 2018.
- [52] E. R. Westervelt, J. W. Grizzle, C. Chevallereau, J. H. Choi, and B. Morris, *Feedback Control of Dynamic Bipedal Robot Locomotion*. CRC Press, 2007.
- [53] K. Aminian, B. Najafi, C. Büla, P. F. Leyvraz, and P. Robert, "Spatio-temporal parameters of gait measured by an ambulatory system using miniature gyroscopes," *Journal of Biomechanics*, vol. 35, no. 5, pp. 689–699, 2002.
- [54] S. Yang and Q. Li, "Inertial sensor-based methods in walking speed estimation: A systematic review," *Sensors (Switzerland)*, vol. 12, no. 5, pp. 6102–6116, 2012.
- [55] K. R. Embry and R. D. Gregg, "Analysis of Continuously Varying Kinematics for Prosthetic Leg Control Applications," *IEEE Trans. Neural Syst. Rehabil. Eng.*, 2020.
- [56] W. Svensson and U. Holmberg, *An autonomous control system for a prosthetic foot ankle*. IFAC, 2006, vol. 4, no. PART 1.
- [57] R. Versluys, P. Beyl, M. V. Damme, A. Desomer, R. V. Ham, and D. Lefeber, "Prosthetic feet: State-of-the-art review and the importance of mimicking human ankle-foot biomechanics," *Disabil. Rehabil. Assist. Tech.*, vol. 4, no. 2, pp. 65–75, 2009.
- [58] M. D. Fox and S. L. Delp, "Contributions of muscles and passive dynamics to swing initiation over a range of walking speeds," *J. Biomech.*, vol. 43, no. 8, 2010.
- [59] A. D. Kuo and J. M. Donelan, "Dynamic principles of gait and their clinical implications," *Phys. Ther.*, vol. 90, 2010.
- [60] N. P. Fey, A. M. Simon, A. J. Young, and L. J. Hargrove, "Controlling Knee Swing Initiation and Ankle Plantarflexion With an Active Prosthesis on Level and Inclined Surfaces at Variable Walking Speeds," *IEEE J. Transl. Eng. Heal. Med.*, vol. 2, no. August, pp. 1–12, 2014.
- [61] A. F. Azocar, L. M. Mooney, J. F. Duval, A. M. Simon, L. J. Hargrove, and E. J. Rouse, "Design and clinical implementation of an open-source bionic leg," *Nat. Biomed. Eng.*, vol. 4, no. 10, pp. 941–953, 2020.
- [62] F. Zhang, M. Liu, and H. Huang, "Effects of locomotion mode recognition errors on volitional control of powered above-knee prostheses," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 23, no. 1, pp. 64–72, 2015.
- [63] J. H. Bowker and A. A. of Orthopaedic Surgeons, *Atlas of limb prosthetics : surgical, prosthetic, and rehabilitation principles*, 2nd ed., J. H. Bowker, Ed. Mosby Year Book, 1992.
- [64] L. Nolan, A. Wit, K. Dudziński, A. Lees, M. Lake, and M. Wychowański, "Adjustments in gait symmetry with walking speed in trans-femoral and trans-tibial amputees," *Gait & Posture*, vol. 17, no. 2, pp. 142–151, 2003.
- [65] K. K. Patterson, W. H. Gage, D. Brooks, S. E. Black, and W. E. McIlroy, "Evaluation of gait symmetry after stroke: A comparison of current methods and recommendations for standardization," *Gait & Posture*, vol. 31, no. 2, pp. 241–246, 2010.
- [66] S. M. Jaegers, J. H. Arendzen, and H. J. de Jongh, "Prosthetic gait of unilateral transfemoral amputees: A kinematic study," *Arch. Phys. Med. Rehabil.*, vol. 76, no. 8, pp. 736–743, 1995.
- [67] S. Hood, M. K. Ishmael, A. Gunnell, K. B. Foreman, and T. Lenzi, "A kinematic and kinetic dataset of 18 above-knee amputees walking at various speeds," *Sci. Data*, vol. 7, no. 1, pp. 1–8, 2020.
- [68] M. B. Popovic, A. Goswami, and H. Herr, "Ground reference points in legged locomotion: Definitions, biological trajectories and control implications," *Int. J. Rob. Res.*, vol. 24, no. 12, pp. 1013–1032, 2005.

- [69] T. Best, C. Welker, E. Rouse, and R. Gregg, "A Virtual Dog Walk with a Robotic Prosthetic Leg," 2021. [Online]. Available: <https://www.youtube.com/watch?v=ozBN2ZxVxxQ>
- [70] A. F. Azocar and E. J. Rouse, "Characterization of Open-loop Impedance Control and Efficiency in Wearable Robots," *IEEE Robot. Autom. Lett.*, vol. 7, no. 2, pp. 4313–4320, 2022.
- [71] J. C. Selinger, S. M. O'Connor, J. D. Wong, and J. M. Donelan, "Humans can continuously optimize energetic cost during walking," *Curr. Biol.*, vol. 25, no. 18, pp. 2452–2456, sep 2015.
- [72] C. S. Simpson, C. G. Welker, S. D. Uhlrich, S. M. Sketch, R. W. Jackson, S. L. Delp, S. H. Collins, J. C. Selinger, and E. W. Hawkes, "Connecting the legs with a spring improves human running economy," *J. Exp. Biol.*, vol. 222, no. 17, sep 2019.
- [73] S. J. Abram, K. L. Poggensee, N. Sánchez, S. N. Simha, J. M. Finley, S. H. Collins, and J. M. Donelan, "General variability leads to specific adaptation toward optimal movement policies," *Current Biology*, vol. 32, no. 10, pp. 2222–2232.e5, 2022.
- [74] M. K. Shepherd and E. J. Rouse, "Comparing Preference of Ankle-Foot Stiffness in Below-Knee Amputees and Prosthetists." *Press. Nat. Sci. Reports*, 2020.
- [75] E. Reznick, K. Embry, and R. D. Gregg, "Predicting Individualized Joint Kinematics over a Continuous Range of Slopes and Speeds," *IEEE RAS EMBS Int. Conf. Biomed. Robot. Biomech.*, pp. 666–672, 2020.
- [76] K. Zhang, J. Luo, W. Xiao, W. Zhang, H. Liu, J. Zhu, Z. Lu, Y. Rong, C. W. De Silva, and C. Fu, "A Subvision System for Enhancing the Environmental Adaptability of the Powered Transfemoral Prosthesis," *IEEE Trans. Cybern.*, vol. 51, no. 6, 2021.
- [77] B. Zhong, R. L. d. Silva, M. Tran, H. Huang, and E. Lobaton, "Efficient environmental context prediction for lower limb prostheses," *IEEE Transactions on Systems, Man, and Cybernetics: Systems*, vol. 52, no. 6, pp. 3980–3994, 2022.
- [78] M. Li, B. Zhong, E. Lobaton, and H. Huang, "Fusion of Human Gaze and Machine Vision for Predicting Intended Locomotion Mode," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 30, pp. 1103–1112, 2022.
- [79] J. Figueiredo, S. P. Carvalho, D. Goncalve, J. C. Moreno, and C. P. Santos, "Daily Locomotion Recognition and Prediction: A Kinematic Data-Based Machine Learning Approach," *IEEE Access*, vol. 8, 2020.
- [80] S. Cheng, E. Bolivar-Nieto, and R. D. Gregg, "Real-Time Activity Recognition with Instantaneous Characteristic Features of Thigh Kinematics," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 29, pp. 1827–1837, 2021.
- [81] M. S. Orendurff, J. A. Schoen, G. C. Bernatz, A. D. Segal, and G. K. Klute, "How humans walk: Bout duration, steps per bout, and rest duration," *J. Rehabil. Res. Dev.*, vol. 45, no. 7, pp. 1077–1090, 2008.
- [82] A. L. Hof, M. G. Gazendam, and W. E. Sinke, "The condition for dynamic stability," *J. Biomech.*, vol. 38, no. 1, pp. 1–8, 2005.
- [83] H. A. Varol, F. Sup, and M. Goldfarb, "Multiclass real-time intent recognition of a powered lower limb prosthesis," *IEEE Trans. Biomed. Eng.*, vol. 57, no. 3, pp. 542–551, 2010.
- [84] L. J. Hargrove, A. J. Young, A. M. Simon, N. P. Fey, R. D. Lipschutz, S. B. Finucane, E. G. Halsne, K. A. Ingraham, and T. A. Kuiken, "Intuitive control of a powered prosthetic leg during ambulation: A randomized clinical trial," *J. Am. Med. Assoc.*, vol. 313, no. 22, pp. 2244–2252, 2015.



T. Kevin Best (Student Member, IEEE) received the B.S. degree in mechanical engineering from the University of Notre Dame, South Bend, IN, USA, in 2018, and the M.S. degree in robotics from the University of Michigan, Ann Arbor, MI, USA, in 2022. He is currently a doctoral candidate with the Locomotor Control Systems Laboratory and the Neurobionics Laboratory in the Robotics Department at the University of Michigan. His research interests include control of robotic systems, optimization, and biomechanics.



Cara Gonzalez Welker (Member, IEEE) received a B.S. in Biomedical and Chemical Engineering from Vanderbilt University in 2014, an M.S. in Mechanical Engineering in 2017 and Ph.D. in Bioengineering in 2021, both from Stanford University. She is currently an Assistant Professor in the Mechanical Engineering Department and Biomedical Engineering program at the University of Colorado Boulder. Her research interests include haptics, biomechanics, robotics, and assistive devices.



Elliott J. Rouse (S'10, M'12, SM'20) received the B.S. degree in mechanical engineering from The Ohio State University, Columbus, OH, USA, in 2007, the M.S. and Ph.D. degrees in biomedical engineering from Northwestern University, Evanston, IL, USA, in 2009 and 2012. Afterwards, he joined the Massachusetts Institute of Technology, Cambridge MA, USA as a postdoctoral fellow until 2014. He is currently an Associate Professor at the University of Michigan, Ann Arbor, MI, USA in the Departments of Robotics and Mechanical Engineering. Prior to joining the University of Michigan, he was faculty at the Shirley Ryan AbilityLab / Northwestern University, Chicago, IL, USA. His research interests include precision machine design, control, biomechanical modeling, psychophysics, and the use of these tools to develop meaningful exoskeletons and robotic prostheses that advance gait, mobility, and quality of life.



Robert D. Gregg (Senior Member, IEEE) received the B.S. degree in electrical engineering and computer sciences from the University of California at Berkeley, Berkeley, CA, USA, in 2006, and the M.S. and Ph.D. degrees in electrical and computer engineering from the University of Illinois at Urbana-Champaign, Champaign, IL, USA, in 2007 and 2010, respectively. He was previously an Assistant Professor with The University of Texas at Dallas, Richardson, TX, USA. In 2019, he joined the Department of Electrical Engineering and Computer Science, University of Michigan, Ann Arbor, MI, USA, as an Associate Professor. He joined the Department of Robotics at the University of Michigan in 2022. His research interests include the control of bipedal locomotion with applications to autonomous and wearable robots.